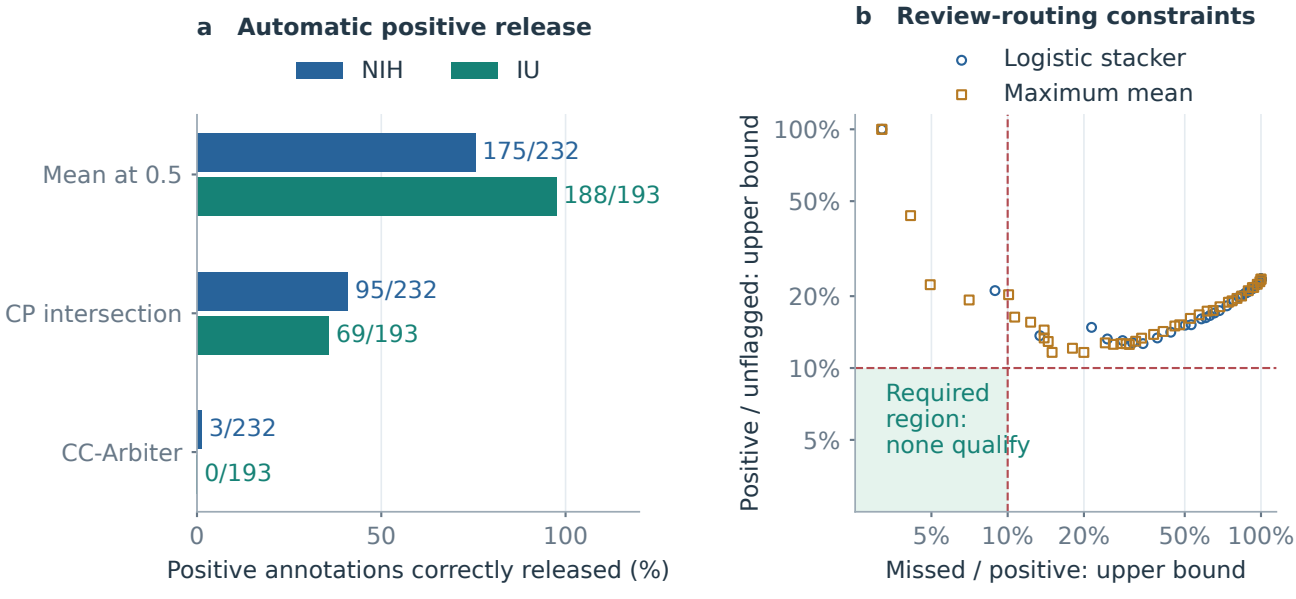

a: seven finding targets. b: any of seven annotations per patient; 1,278 calibration patients. No threshold passed both bounds; both rules flagged all 1,279 test patients.