


Ash-Matrix Pb Calibration (ICP-MS Validated)

PELLET
 $R^2 = 0.886$, $n = 32$
LOD = 197 ppm



POWDER
 $R^2 = 0.714$, $n = 24$
LOD = 242 ppm

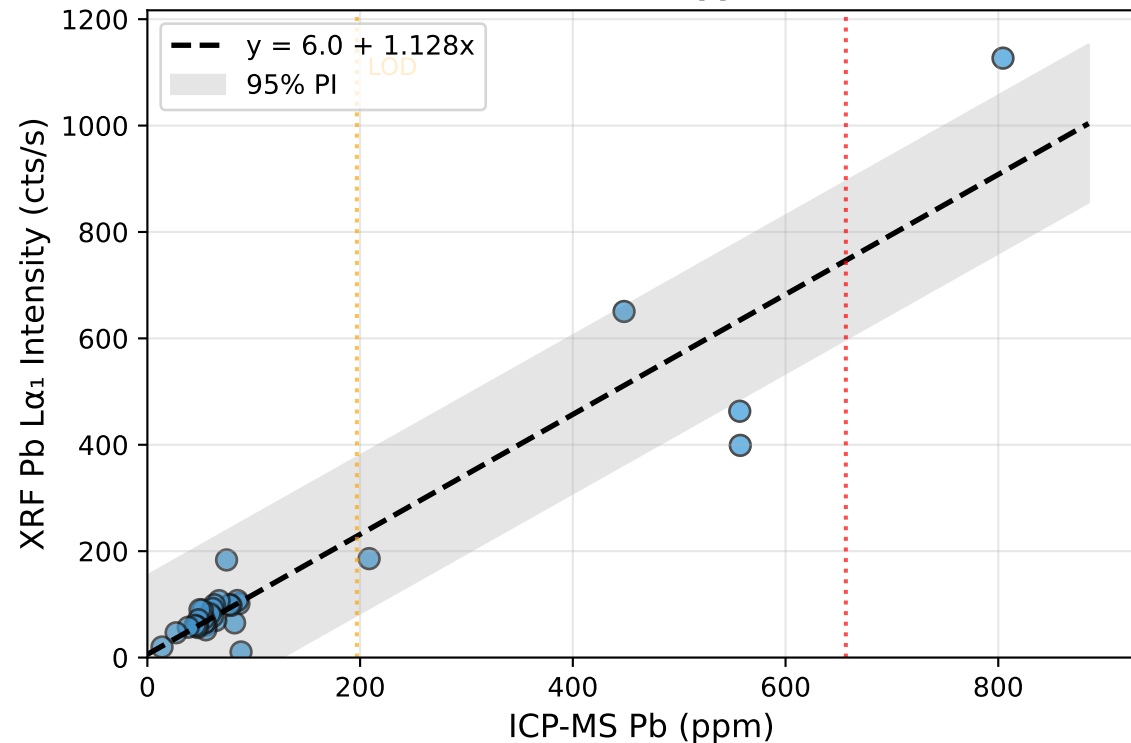