



PBP Clay Standards: Refined Calibration (n=23, excl. mislabeled sample)


A. FP Concentration vs Known

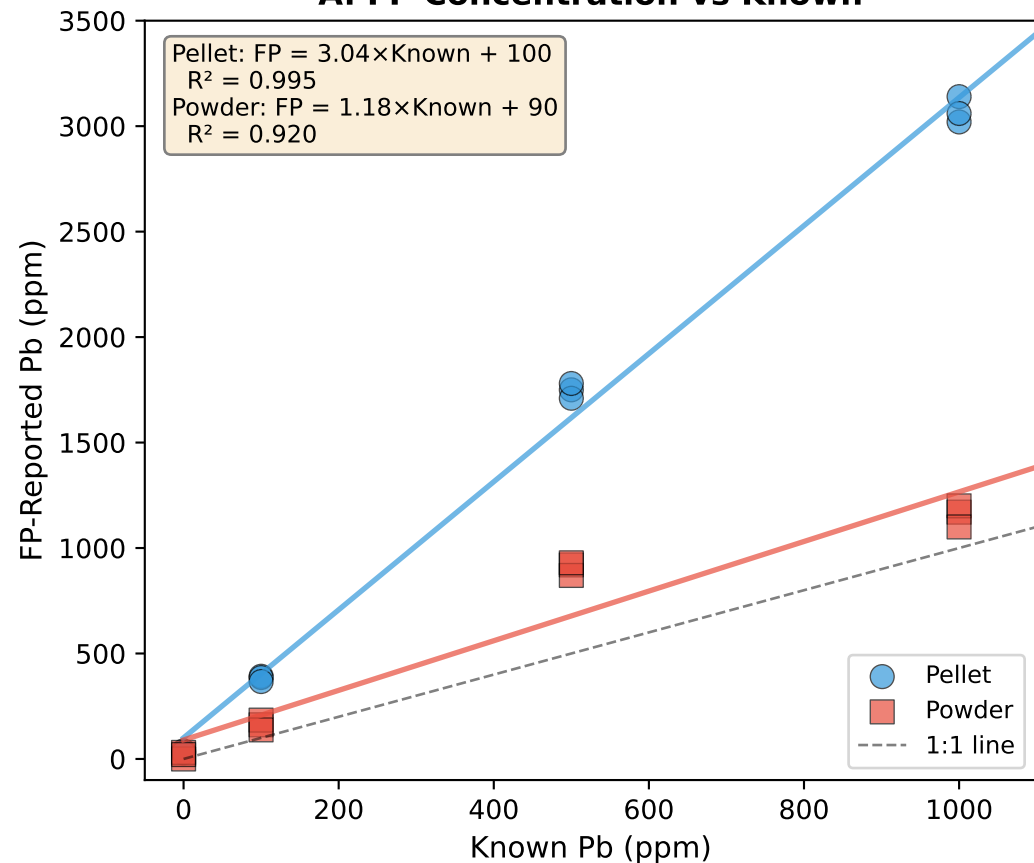

B. Emission Intensity vs Known

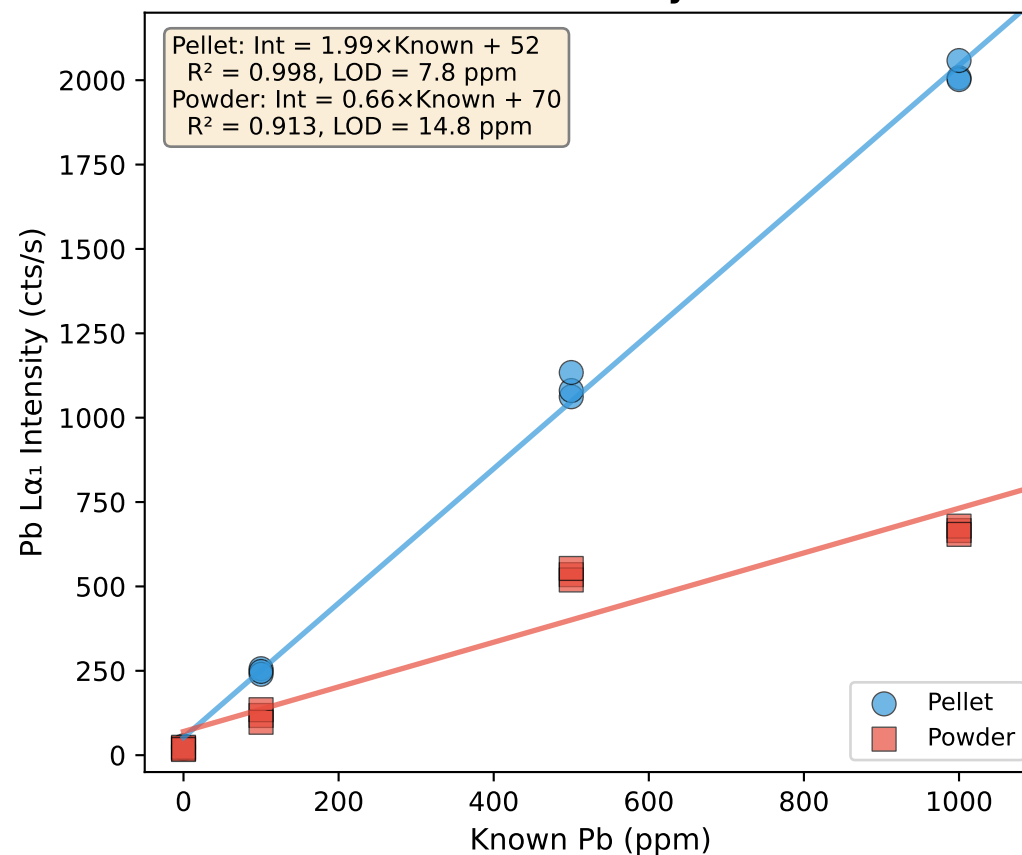

C. Intensity Calibration Residuals

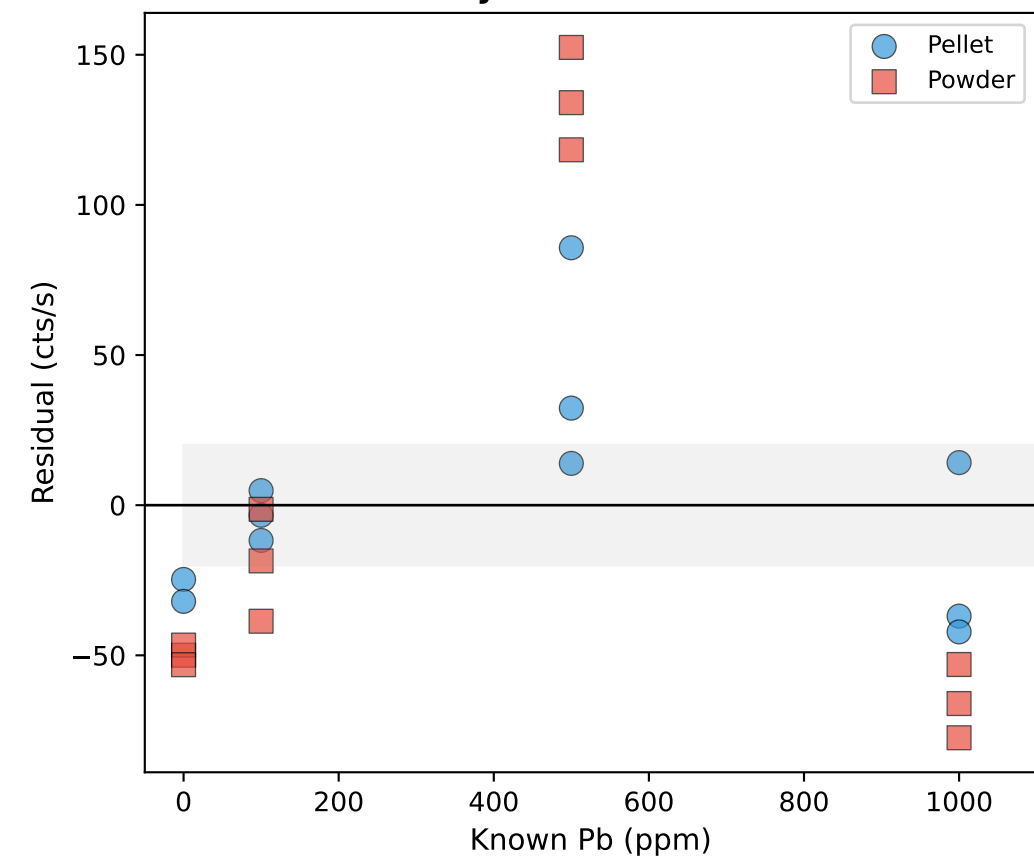

D. PBP04 Blank Measurements

