


XRF vs ICP-MS Validation (Ash-Matrix Calibration)

PELLET - Validation
CV-RMSE = 101 ppm



POWDER - Validation
CV-RMSE = 177 ppm

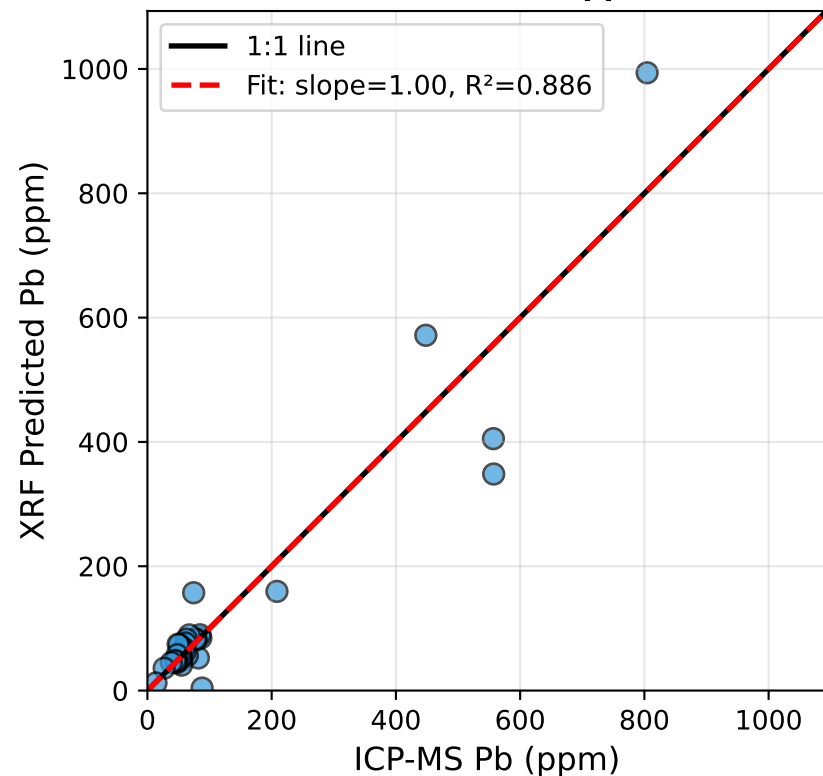