


Calibration: PBP clay standards (4 arms)


pellet_FP

response = FP_concentration
 $R^2 = 0.995$, RMSE = 27.6 ppm, n = 12

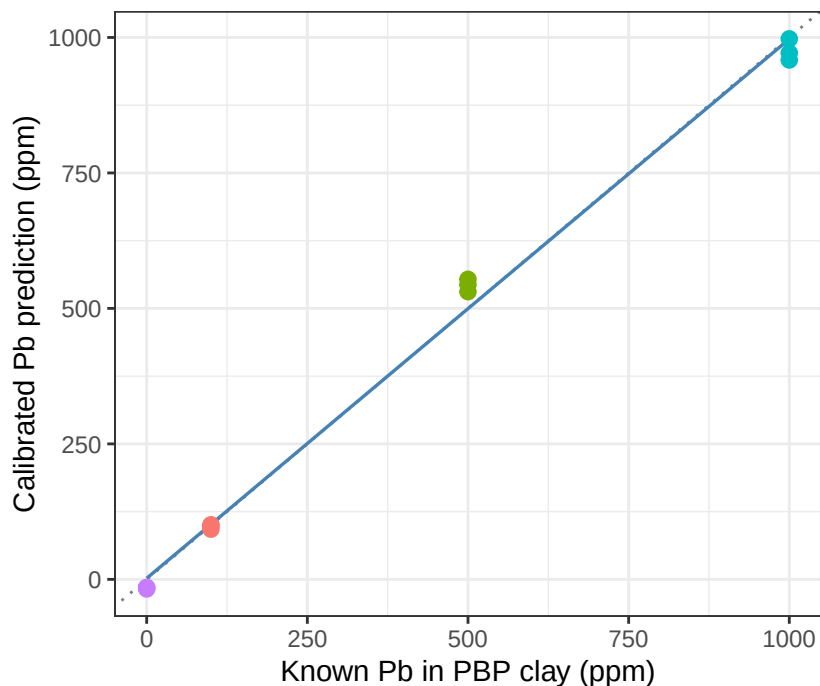


pellet_intensity

response = Pb_Lb1,Lb2 (multi)
 $R^2 = 0.999$, RMSE = 14.4 ppm, n = 12

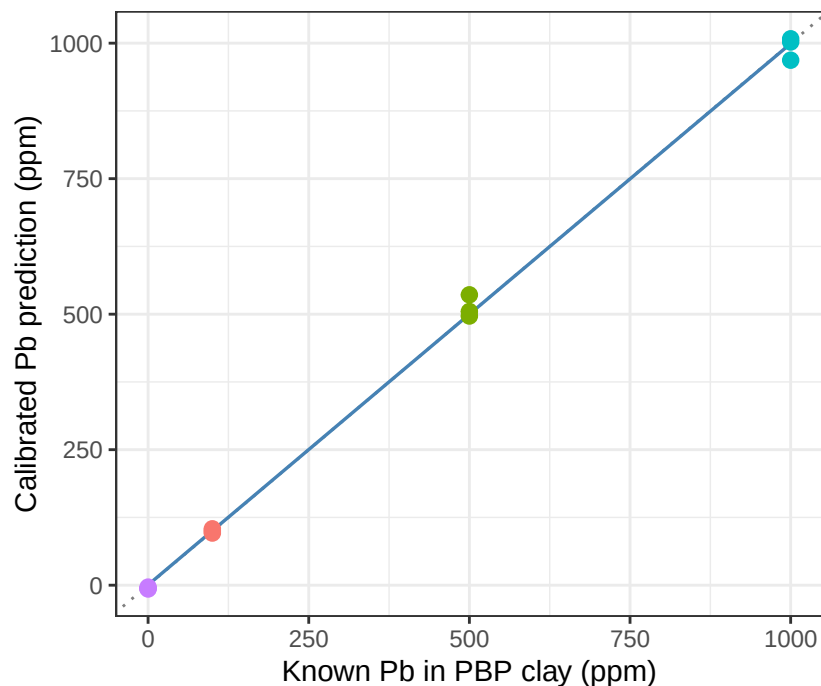

powder_FP

response = FP_concentration
 $R^2 = 0.913$, RMSE = 115.6 ppm, n = 11

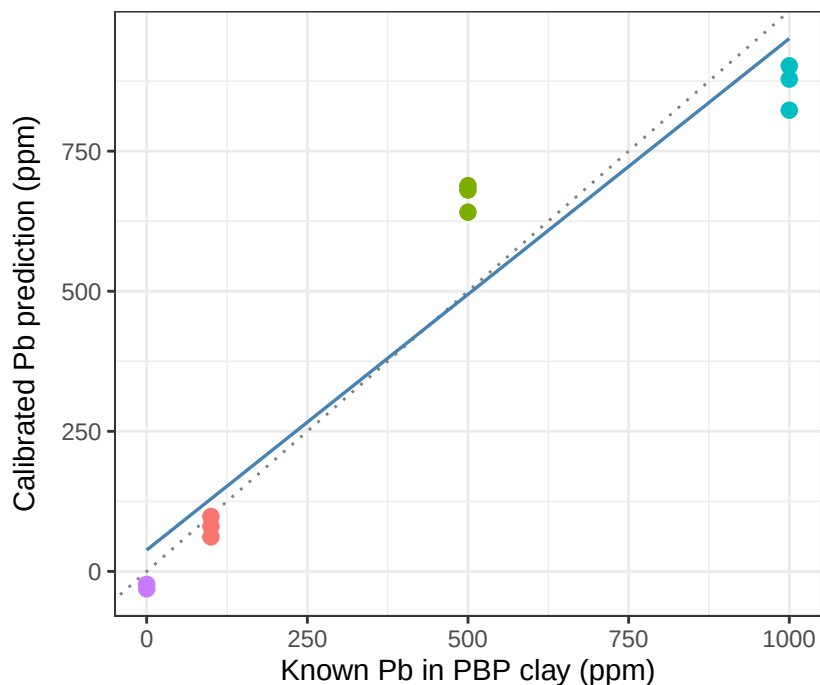

powder_intensity

response = Pb_Lb1,Lb3 (multi)
 $R^2 = 0.937$, RMSE = 97.9 ppm, n = 11

