


Emission Intensity Calibration: Predicted Pb vs ICP-MS Reference

A. Pellet Preparation



B. Powder Preparation

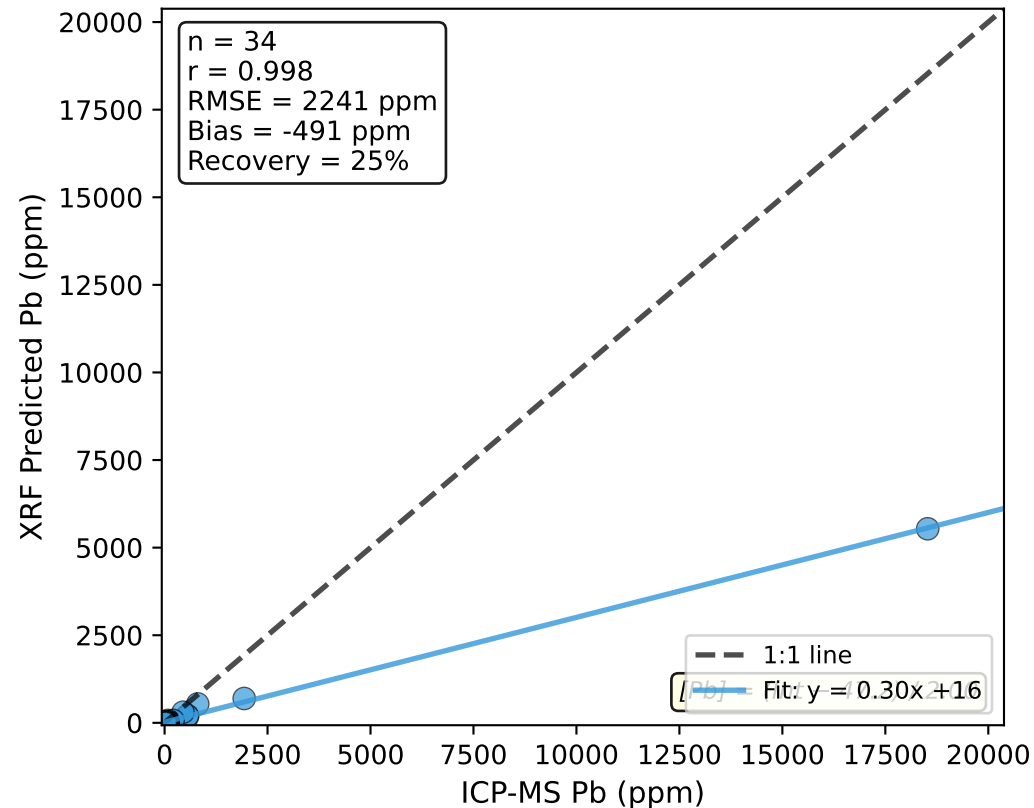