(a)

Art. 7(2) duty

Member States shall take all appropriate measures to ensure that measuring instruments are made available on the market and/or put into use only if they satisfy this Directive

↓

Annex I requirement

the error of measurement shall not exceed the instrument-specific maximum permissible error

This is the structure the predicate searches for.

“all appropriate measures” is the same form the predicate treats as a hedge elsewhere and did not catch here.

The Directive returns 1 provision and the audit confirms 0. The corpus therefore holds no verified positive control: this is the legal form, not a confirmed instance of it.

(b)

Article 2(1) enumerates 10 instrument categories

- **MI-001** water meters
- **MI-002** gas meters and volume conversion devices
- **MI-003** active electrical energy meters
- **MI-004** thermal energy meters
- **MI-005** measuring systems for continuous and dynamic…
- **MI-006** automatic weighing instruments
- **MI-007** taximeters
- **MI-008** material measures
- **MI-009** dimensional measuring instruments
- **MI-010** exhaust gas analysers

None is a law-enforcement measuring instrument, a CBRN detector, an airborne sensing payload, or any instrument whose reading supports a police determination.

(c)

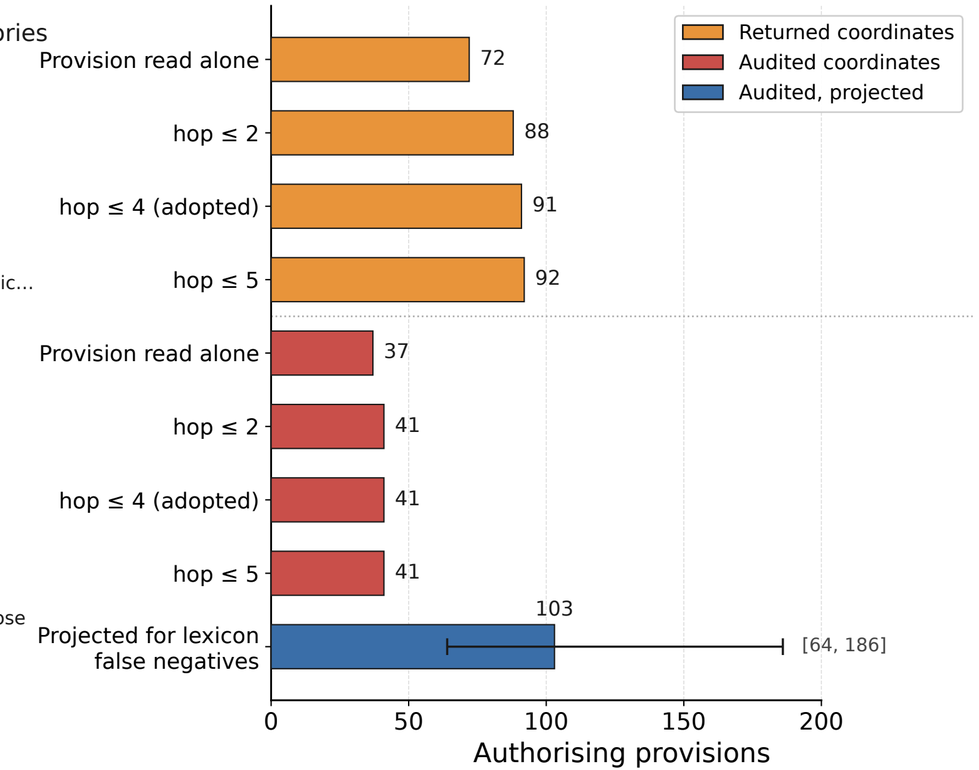

The two blocks are not added: the lexicon projection estimates missed bindings and therefore applies to the audited count, not to what the predicate returns. The interval is the Wilson interval of the false-negative rate carried onto that projection.