A single-conformer harmonic DFT library does not replace measured reference spectra

Eleven vials of authentic chemical warfare agent · 1064 nm · identical pipeline, grid and metric; only the library differs

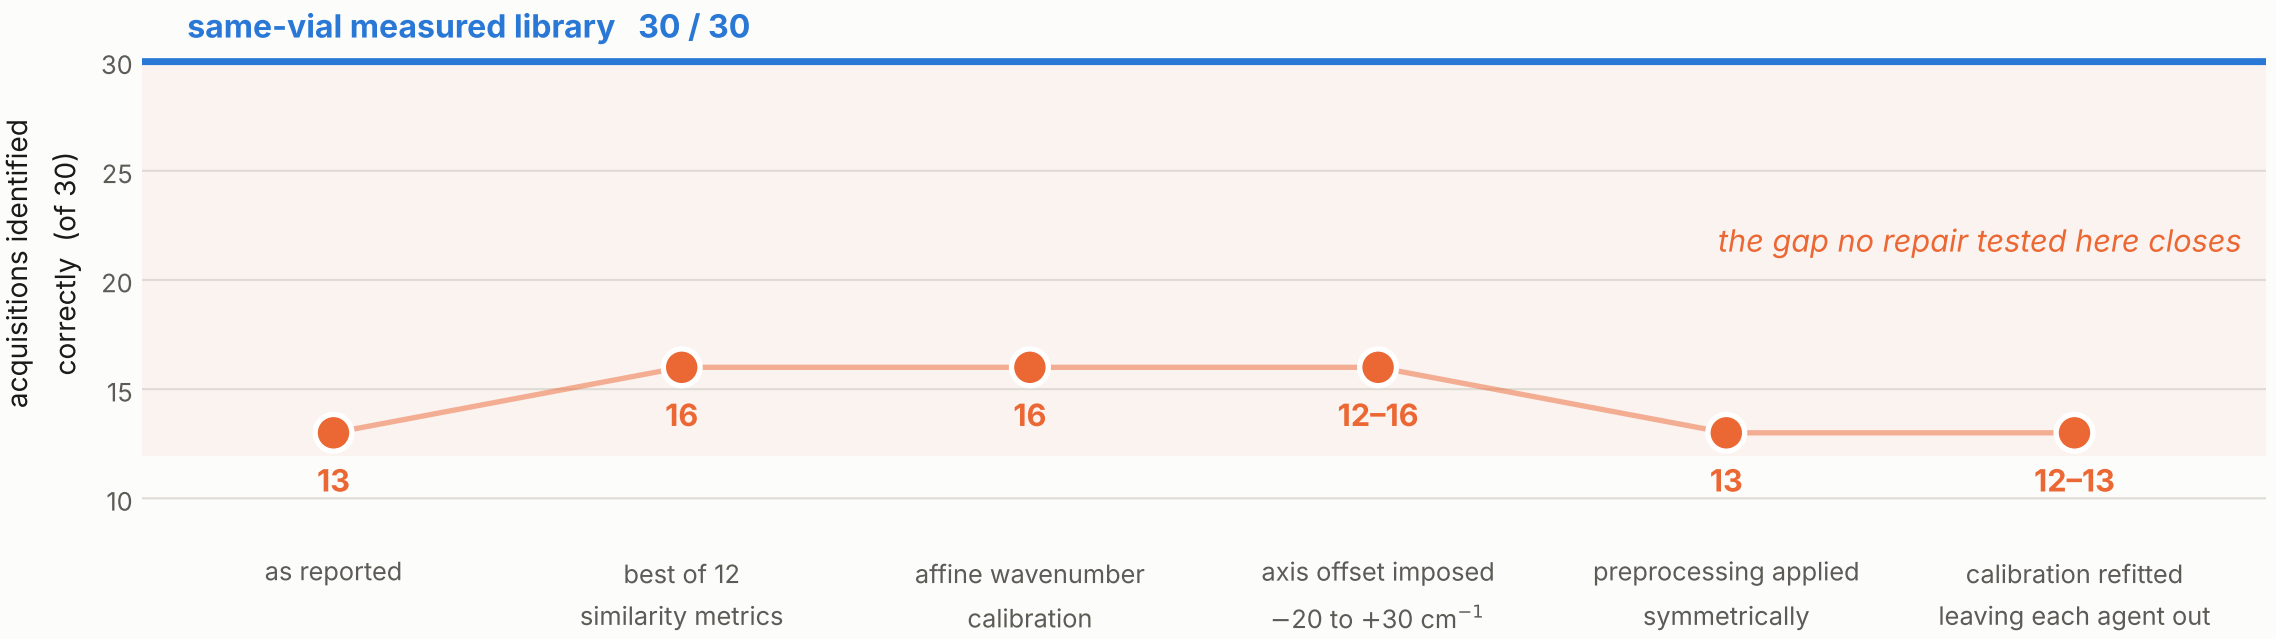

Every entry is the same thirty acquisitions under the same metric, after two wrong computed structures were corrected.