Data File C:\Users\P...s\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30\F-067-67-S2-1-1.D
Sample Name: S2-1-1

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   67
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   67   (F)
Injection Date  : 3/3/2025 11:55:02 PM                Inj :    1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
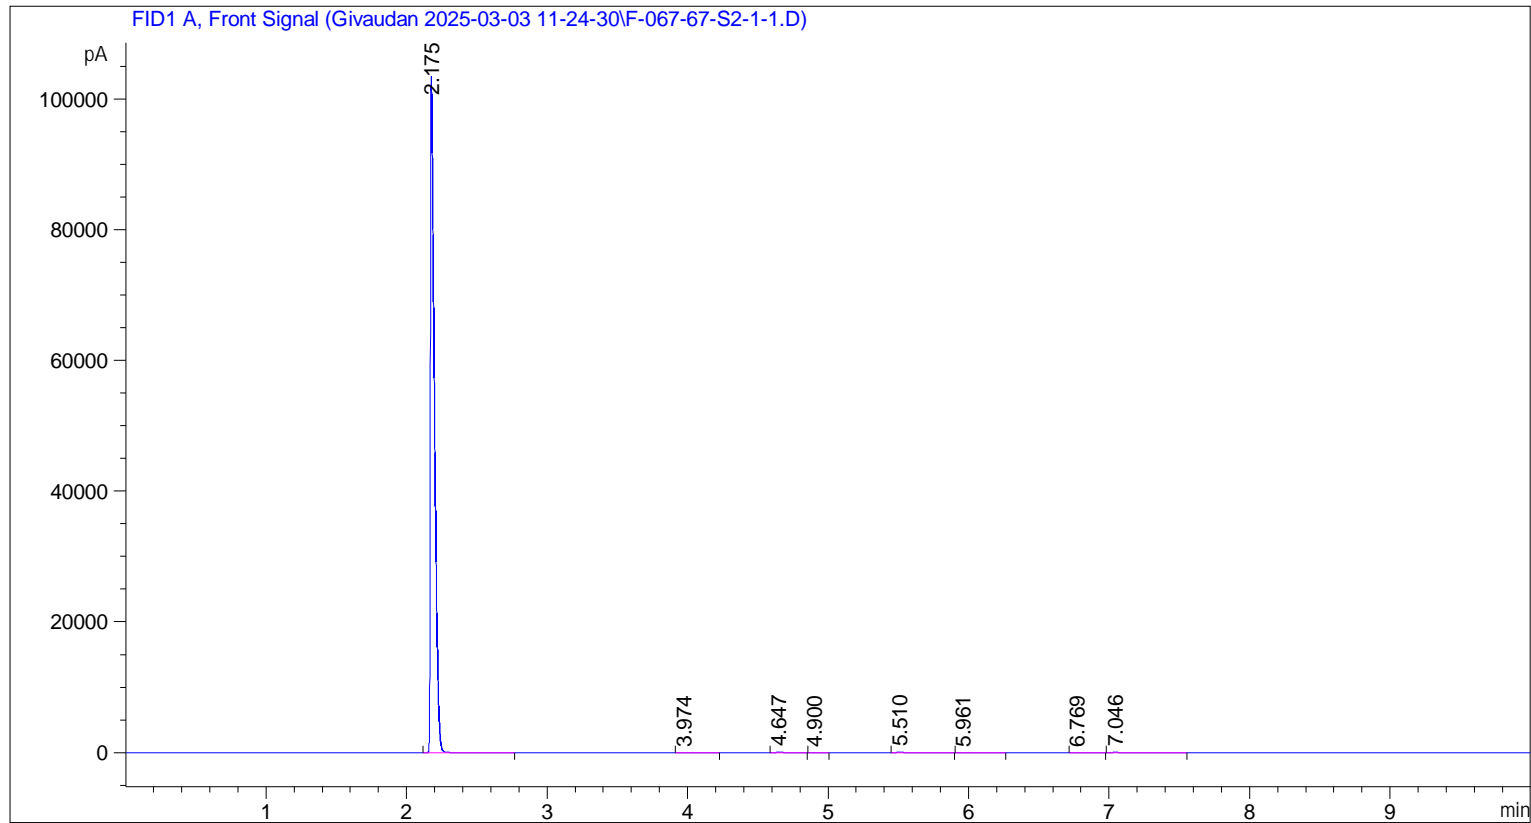

FID1 A, Front Signal (Givaudan 2025-03-03 11-24-30\F-067-67-S2-1-1.D)

```
=====================================================================
                      Area Percent Report
=====================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]   [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
   1   2.175 BB      0.0290 2.06074e5  99.78009 ?
   2   3.974 BB      0.0404   38.07378  0.01844 Acetate
   3   4.647 BB      0.0388  147.64432  0.07149 Propionate
   4   4.900 BB      0.0350    4.91757  0.00238 Isobutyrate
   5   5.510 BB      0.0397  145.77057  0.07058 Butyrate
   6   5.961 BB      0.0379    6.60229  0.00320 Isovaleric
   7   6.769 BB      0.0426    9.20100  0.00446 Valeric
   8   7.046 BB      0.0372  101.97375  0.04938 InternalSD
```

```
  Peak RetTime  Type   Width     Area       Area     Name
   #   [min]          [min]    [pA*s]       %
----|-------|------|-------|----------|--------|--------------------
Totals :                     2.06528e5
```

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                        *** End of Report ***