Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16\F-003-3-GD_P1_B2.D
Sample Name: GD_P1_B2

```
========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   3
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   3   (F)
Injection Date  : 1/23/2025 4:10:38 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
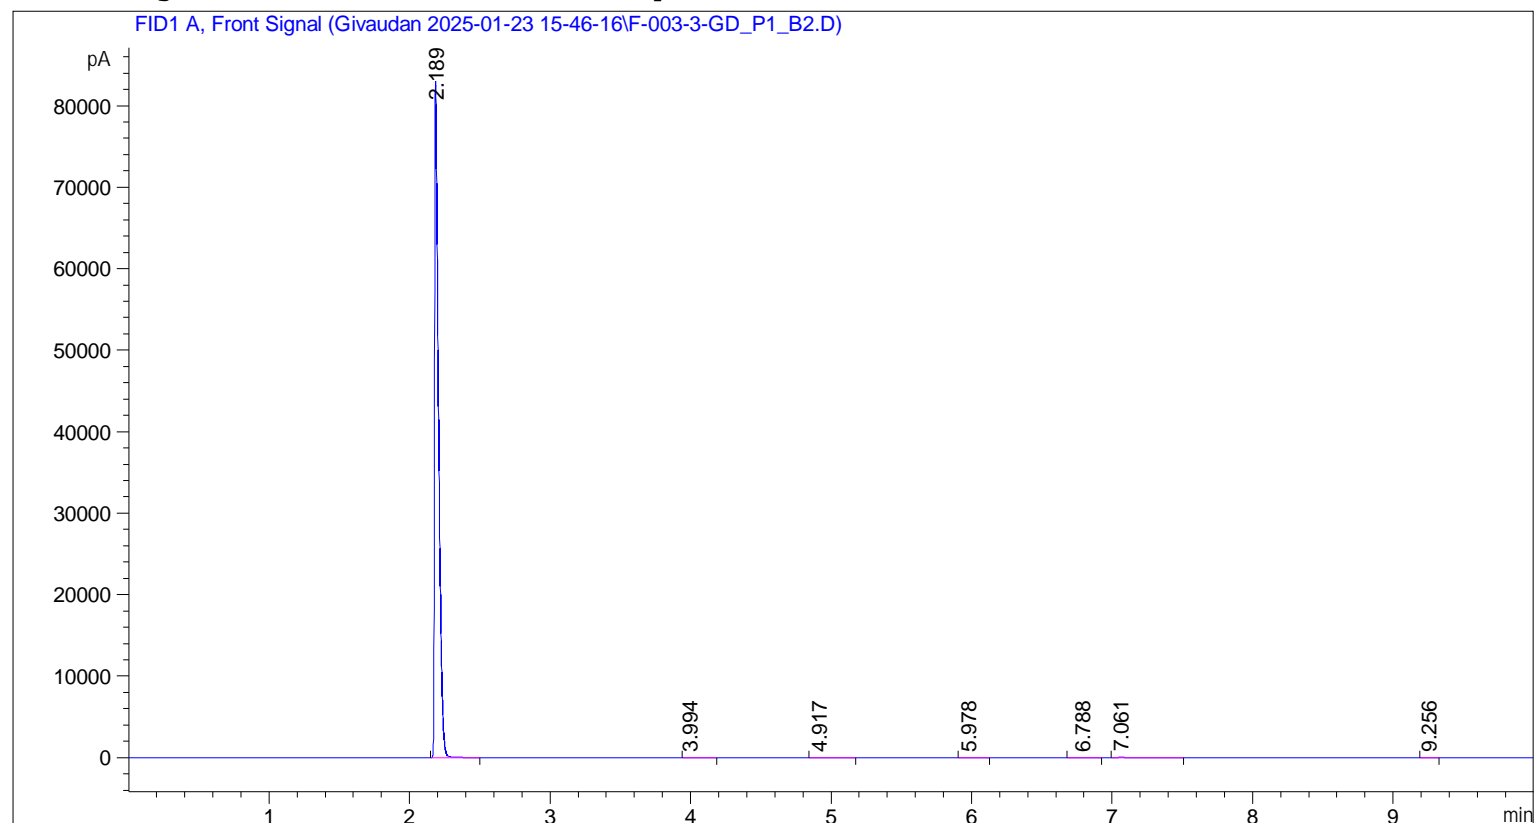

FID1 A, Front Signal (Givaudan 2025-01-23 15-46-16\F-003-3-GD_P1_B2.D)

```
========================================================================
                    Area Percent Report
========================================================================


Sorted By            :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier           :       1.0000
Dilution             :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area       Name
  #   [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   2.189 BB      0.0288 1.61126e5  99.90715 ?
   2   3.994 BB      0.0399   25.07020  0.01554 Acetate
   3   4.725         0.0000    0.00000  0.00000 Propionate
   4   4.917 BB      0.0334    7.65663  0.00475 Isobutyrate
   5   5.598         0.0000    0.00000  0.00000 Butyrate
   6   5.978 BB      0.0341    8.88096  0.00551 Isovaleric
   7   6.788 BB      0.0361    8.50123  0.00527 Valeric
   8   7.061 BB      0.0335   94.28277  0.05846 InternalSD
```

```
Peak RetTime  Type   Width     Area       Area      Name
  #    [min]         [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
  9   9.256 BB      0.0376    5.34850  0.00332 ?


Totals :                     1.61275e5
```

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                       *** End of Report ***