Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30\F-071-71-S2-20-2.D
Sample Name: S2-20-2

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  71
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                          Location :   71  (F)
Injection Date  : 3/4/2025 12:40:20 AM                 Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```

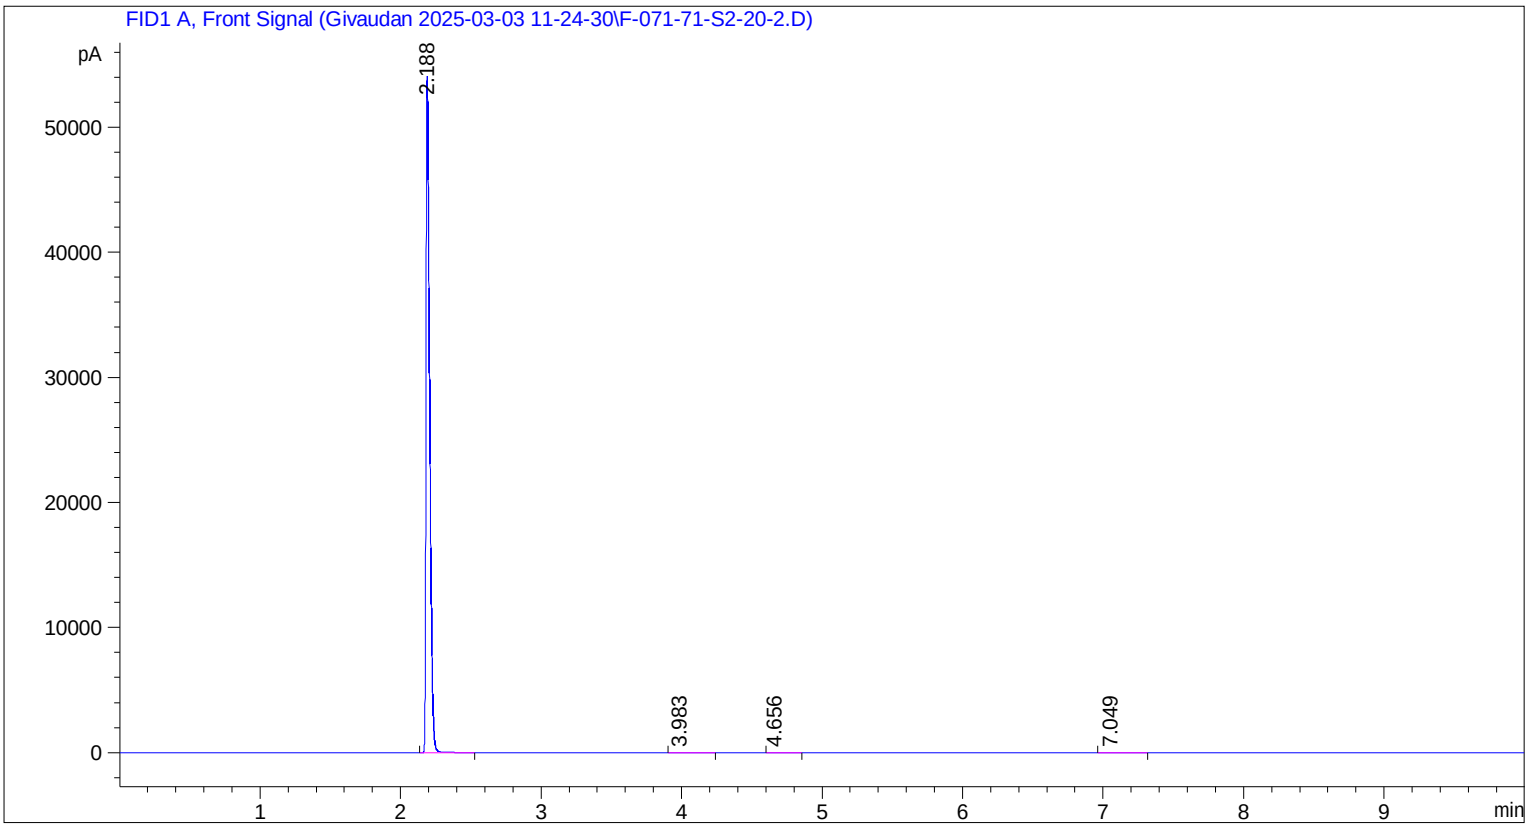


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      9/13/2021 3:53:03 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|---------------------
   1   2.188 BB      0.0273 9.64631e4  99.96400 ?
   2   3.983 BB      0.0442   12.23801  0.01268 Acetate
   3   4.656 BB      0.0434    6.43756  0.00667 Propionate
   4   4.978         0.0000    0.00000  0.00000 Isobutyrate
   5   5.598         0.0000    0.00000  0.00000 Butyrate
   6   6.050         0.0000    0.00000  0.00000 Isovaleric
   7   6.869         0.0000    0.00000  0.00000 Valeric
   8   7.049 BB      0.0401   16.05998  0.01664 InternalSD
```

Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30\F-071-71-S2-20-2.D
Sample Name: S2-20-2

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
Totals :				9.64978e4		

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

==========

*** End of Report ***