Data File C:\Users\P...nts\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30\F-019-19-FS-2.D
Sample Name: FS-2

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :  19
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   19  (F)
Injection Date  : 3/3/2025 2:51:13 PM                Inj :   1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
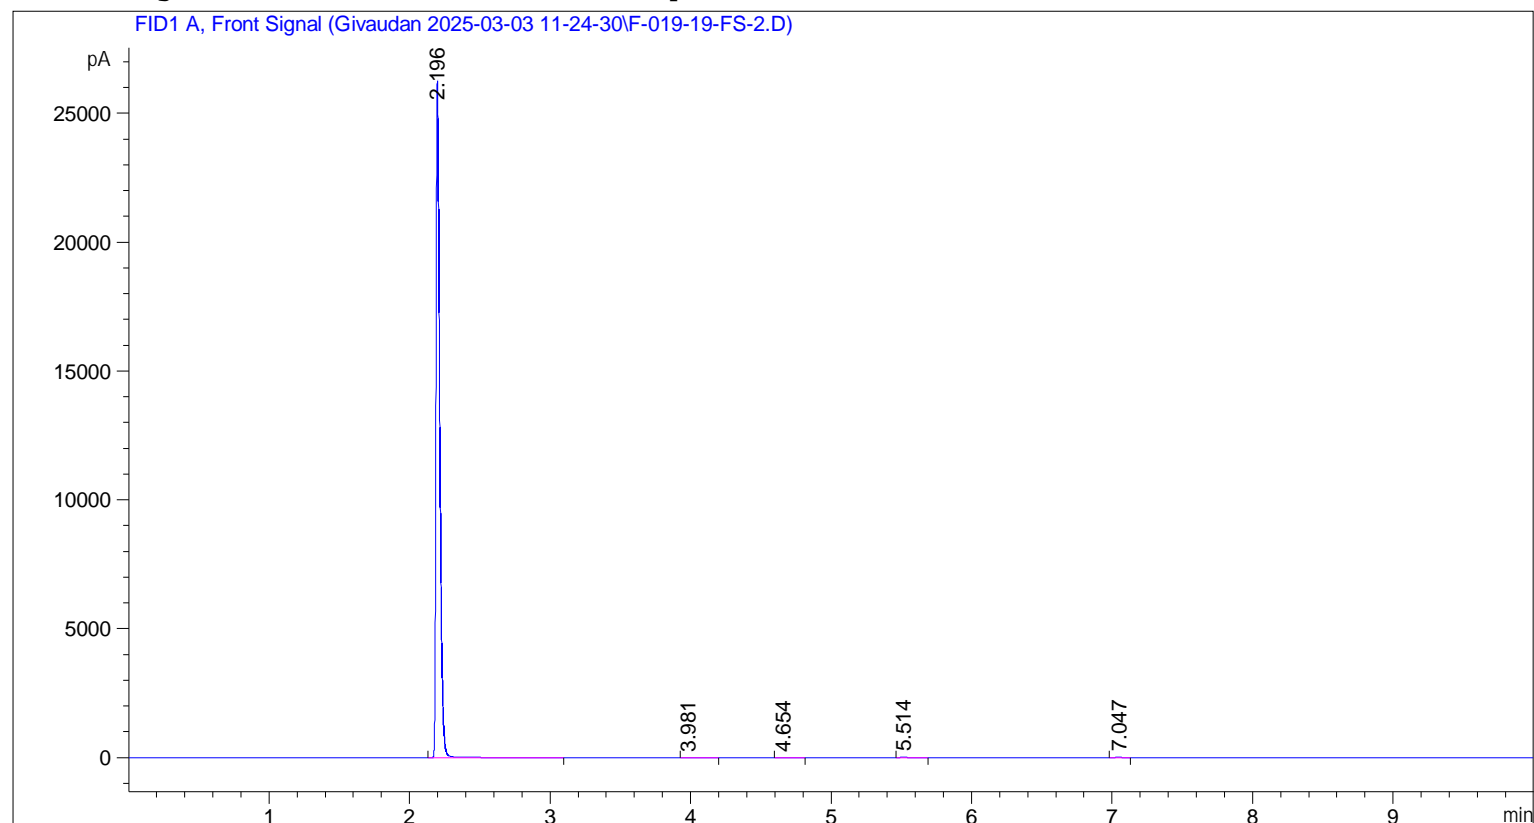

FID1 A, Front Signal (Givaudan 2025-03-03 11-24-30\F-019-19-FS-2.D)

```
=====================================================================
                    Area Percent Report
=====================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area       Area     Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
  1   2.196 BB      0.0279 4.82172e4  99.82357 ?
  2   3.981 BB      0.0399    9.76861  0.02022 Acetate
  3   4.654 BB      0.0384   10.10540  0.02092 Propionate
  4   4.978         0.0000    0.00000  0.00000 Isobutyrate
  5   5.514 BB      0.0372   42.54538  0.08808 Butyrate
  6   6.050         0.0000    0.00000  0.00000 Isovaleric
  7   6.869         0.0000    0.00000  0.00000 Valeric
  8   7.047 BB      0.0347   22.80076  0.04720 InternalSD
```

```
  Peak RetTime  Type   Width     Area       Area     Name
   #   [min]           [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
Totals :                    4.83025e4
```

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

=========================================================================
                        *** End of Report ***