```
========================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   8
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   8   (F)
Injection Date  : 1/23/2025 5:07:15 PM               Inj :   1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
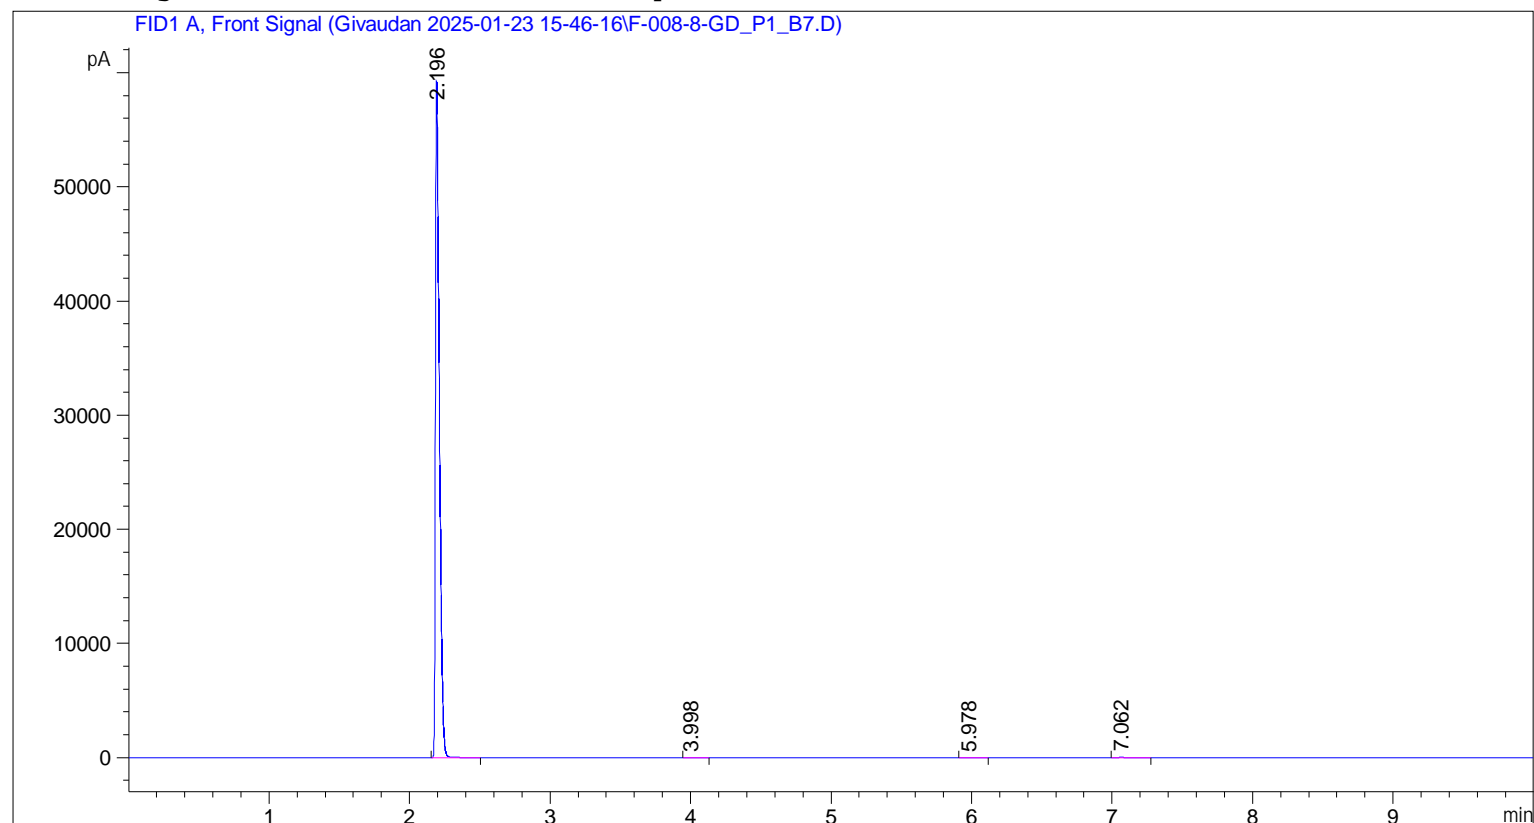

FID1 A, Front Signal (Givaudan 2025-01-23 15-46-16\F-008-8-GD_P1_B7.D)

```
========================================================================
                     Area Percent Report
========================================================================


Sorted By             :       Signal
Calib. Data Modified  :       9/13/2021 3:53:03 PM
Multiplier            :       1.0000
Dilution              :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   2.196 BB      0.0285 1.14188e5  99.95441 ?
   2   3.998 BB      0.0409   10.30256  0.00902 Acetate
   3   4.725         0.0000    0.00000  0.00000 Propionate
   4   4.978         0.0000    0.00000  0.00000 Isobutyrate
   5   5.598         0.0000    0.00000  0.00000 Butyrate
   6   5.978 BB      0.0356    3.72780  0.00326 Isovaleric
   7   6.869         0.0000    0.00000  0.00000 Valeric
   8   7.062 BB      0.0346   38.05291  0.03331 InternalSD
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
Totals :				1.14240e5		

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                          *** End of Report ***