Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16\F-006-6-GD_P1_A5.D
Sample Name: GD_P1_A5

```
========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   6
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   6  (F)
Injection Date  : 1/22/2025 1:11:27 PM                 Inj :   1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
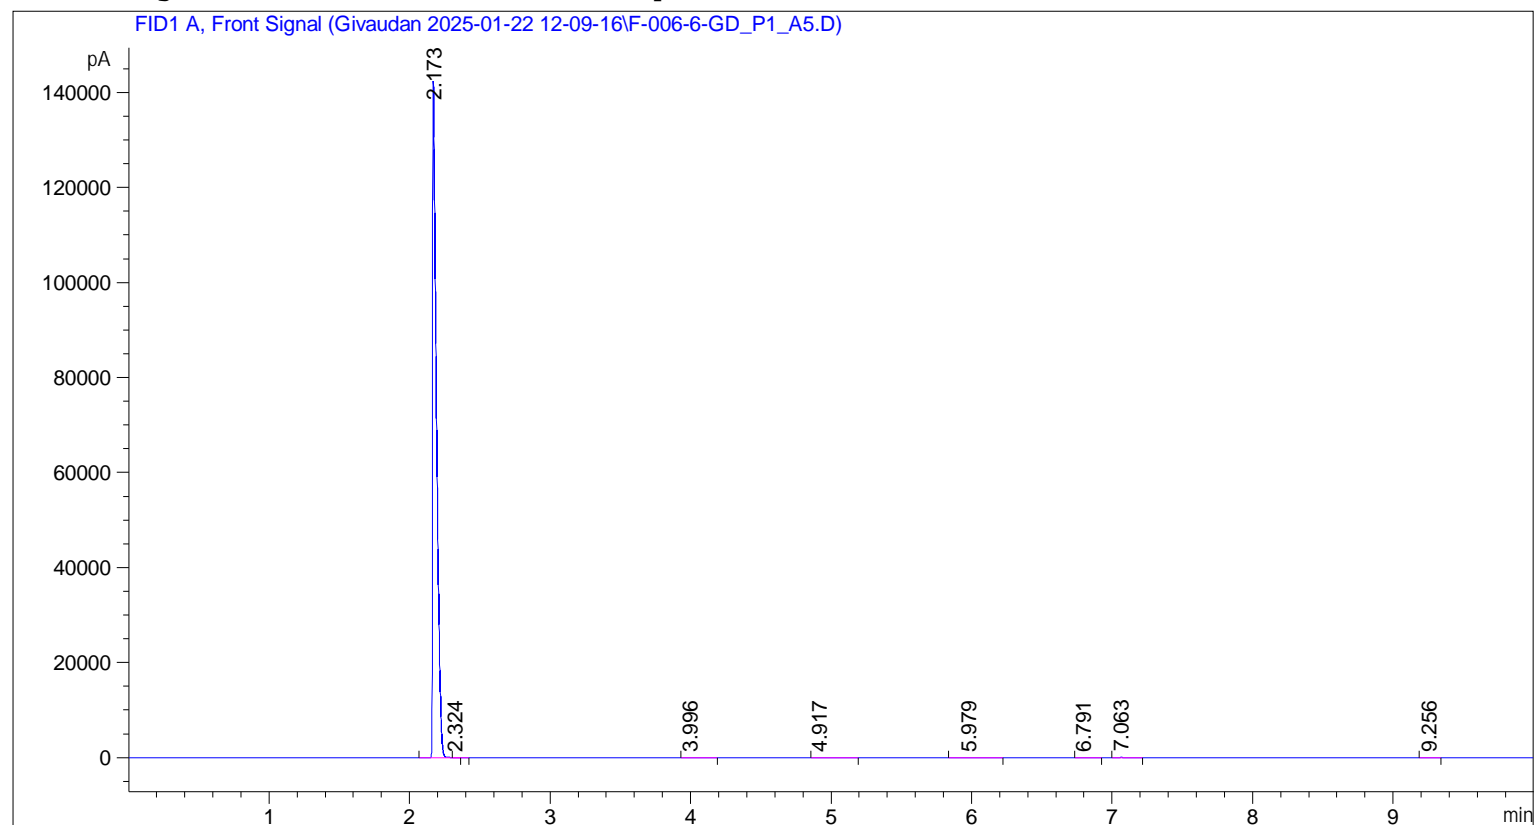

FID1 A, Front Signal (Givaudan 2025-01-22 12-09-16\F-006-6-GD_P1_A5.D)

```
========================================================================
                        Area Percent Report
========================================================================

Sorted By            :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier           :       1.0000
Dilution             :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

```
Peak RetTime  Type   Width     Area        Area      Name
 #    [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
  1   2.173 BB S   0.0272 2.72390e5  99.95073 ?
  2   2.324 BB T   0.0314    8.68292  0.00319 ?
  3   3.996 BB     0.0426   24.30460  0.00892 Acetate
  4   4.725        0.0000    0.00000  0.00000 Propionate
  5   4.917 BB     0.0340    6.19216  0.00227 Isobutyrate
  6   5.598        0.0000    0.00000  0.00000 Butyrate
  7   5.979 BB     0.0529   21.10275  0.00774 Isovaleric
  8   6.791 BB     0.0367    6.98945  0.00256 Valeric
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.063	BB	0.0347	62.94917	0.02310	InternalSD
10	9.256	BB	0.0371	4.05910	0.00149	?

Totals :   2.72524e5

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                        *** End of Report ***