Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30\F-072-72-S2-13-3.D
Sample Name: S2-13-3

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  72
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   72  (F)
Injection Date  : 3/4/2025 12:51:41 AM                  Inj :   1
                                                  Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
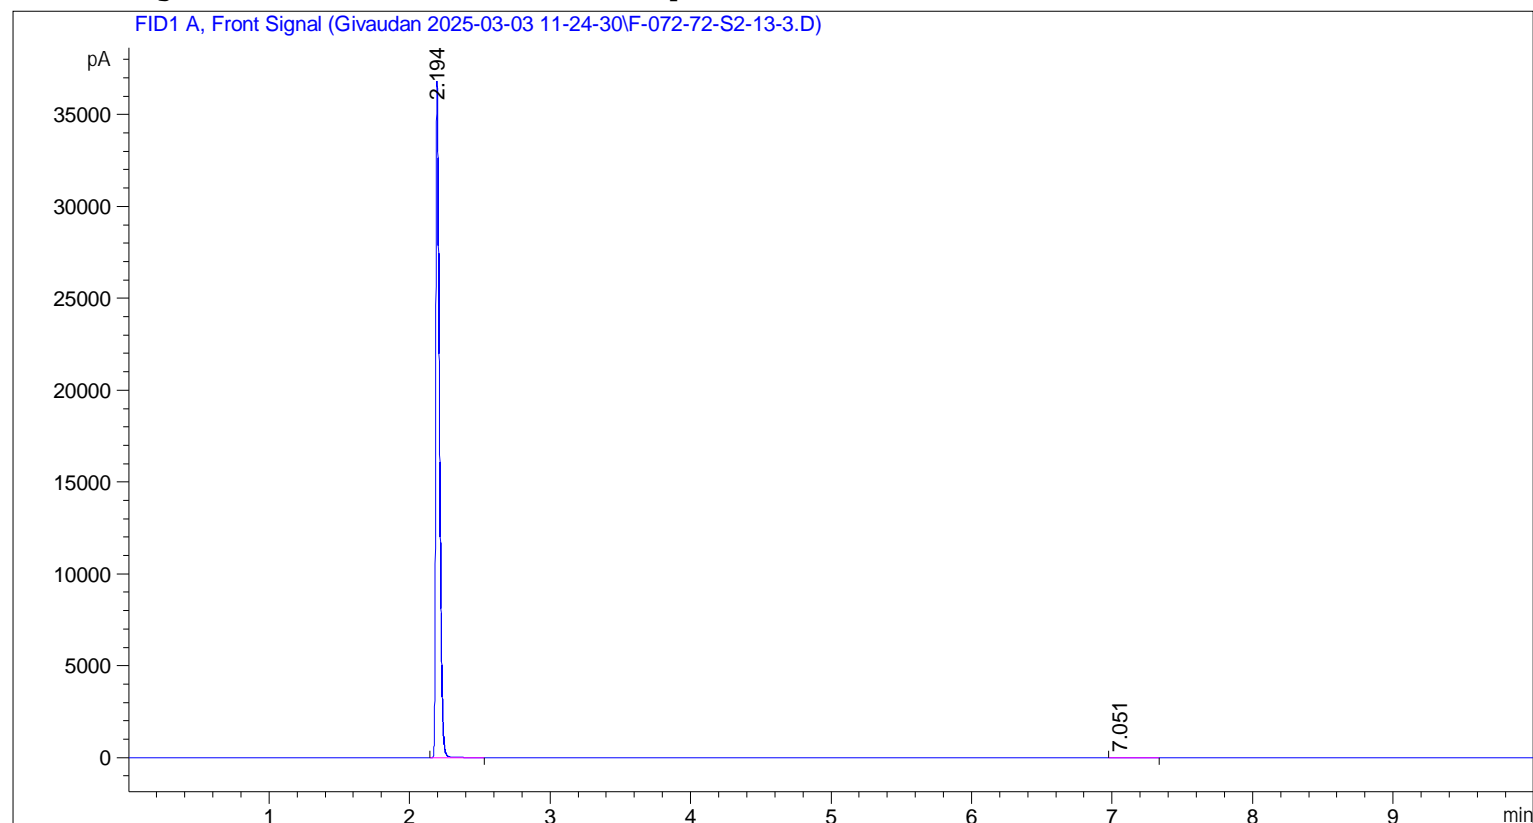

FID1 A, Front Signal (Givaudan 2025-03-03 11-24-30\F-072-72-S2-13-3.D)

```
=====================================================================
                     Area Percent Report
=====================================================================


Sorted By             :        Signal
Calib. Data Modified  :        9/13/2021 3:53:03 PM
Multiplier            :        1.0000
Dilution              :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area       Area      Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   2.194 BB      0.0275 6.64787e4  99.98400 ?
   2   4.042         0.0000   0.00000  0.00000 Acetate
   3   4.725         0.0000   0.00000  0.00000 Propionate
   4   4.978         0.0000   0.00000  0.00000 Isobutyrate
   5   5.598         0.0000   0.00000  0.00000 Butyrate
   6   6.050         0.0000   0.00000  0.00000 Isovaleric
   7   6.869         0.0000   0.00000  0.00000 Valeric
   8   7.051 BB      0.0434  10.63787  0.01600 InternalSD
```

```
   Peak RetTime  Type   Width     Area      Area     Name
     #   [min]          [min]    [pA*s]       %
   ----|-------|------|-------|----------|--------|--------------------
   Totals :                    6.64893e4
```

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

```
=========================================================================
                          *** End of Report ***
```