


```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    1
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                     Location  :    1 (F)
Injection Date  : 1/23/2025 3:47:58 PM        Inj       :    1
                                           Inj Volume: 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
=====
```

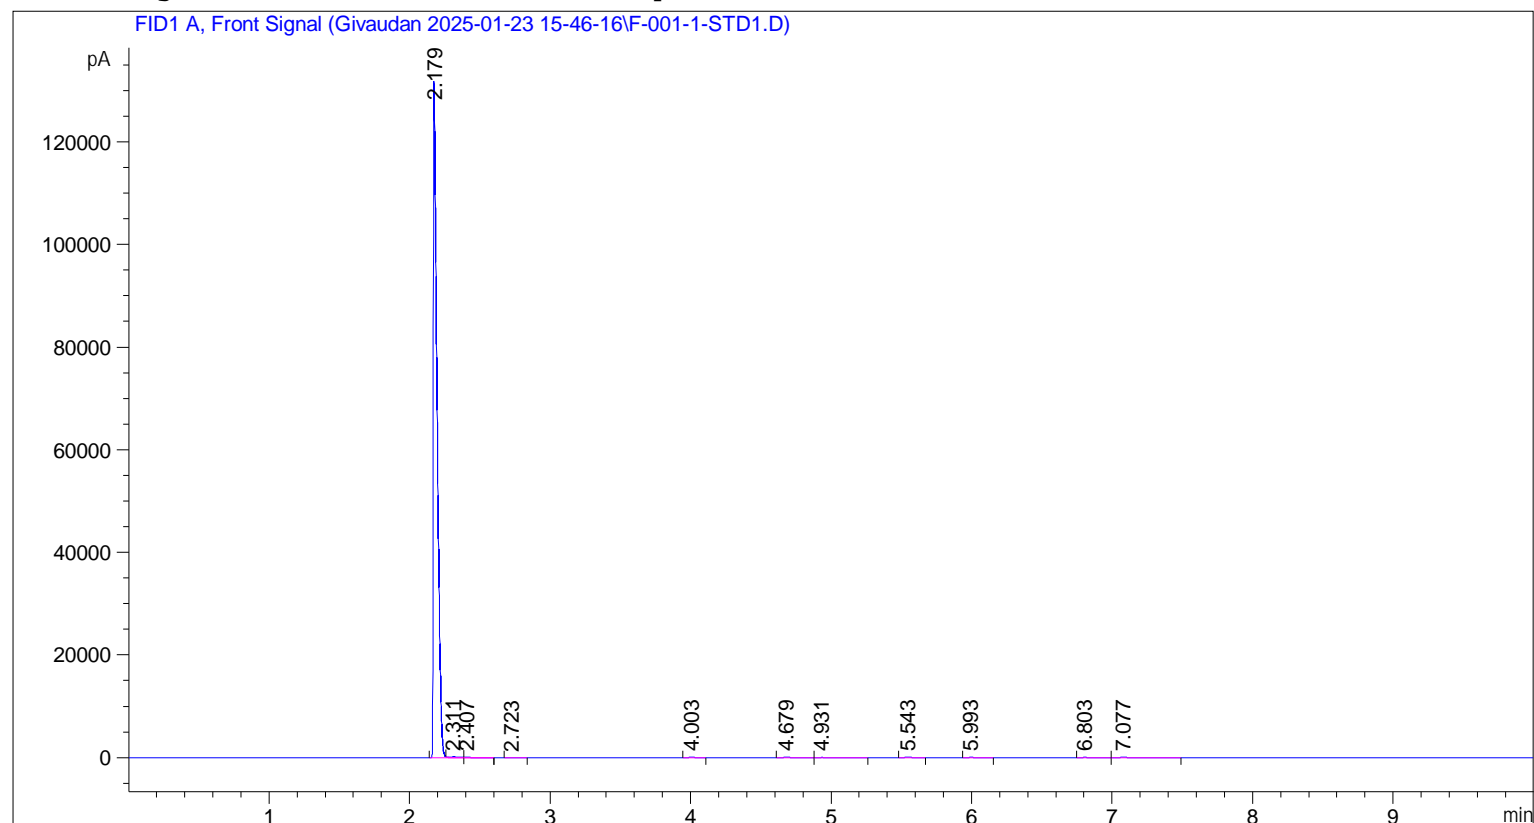

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.179	BV R	0.0284	2.47506e5	99.34572	?
2	2.311	VV E	0.0563	672.35468	0.26987	?
3	2.407	VB E	0.0521	141.55258	0.05682	?
4	2.723	BB	0.0502	16.75622	0.00673	?
5	4.003	BB	0.0385	115.64174	0.04642	Acetate
6	4.679	BV	0.0363	152.08679	0.06105	Propionate
7	4.931	VB	0.0337	50.67844	0.02034	Isobutyrate
8	5.543	BB	0.0334	169.10625	0.06788	Butyrate

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	5.993	BB	0.0342	75.14791	0.03016	Isovaleric
10	6.803	BB	0.0338	68.96566	0.02768	Valeric
11	7.077	BB	0.0333	167.74976	0.06733	InternalSD

Totals : 2.49136e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====
*** End of Report ***