```
=====================================================================
Acq. Operator   : SYSTEM                         Seq. Line :   6
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                          Location :   6  (F)
Injection Date  : 4/16/2025 4:13:05 PM               Inj :   1
                                               Inj Volume : 1 µl
Sequence File   : C:\Users\Public\Documents\ChemStation\2\Data\std 2025-04-16 15-15-06\std.S
Method          : C:\Users\Public\Documents\ChemStation\2\Data\std 2025-04-16 15-15-06\SCFA_
                  FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
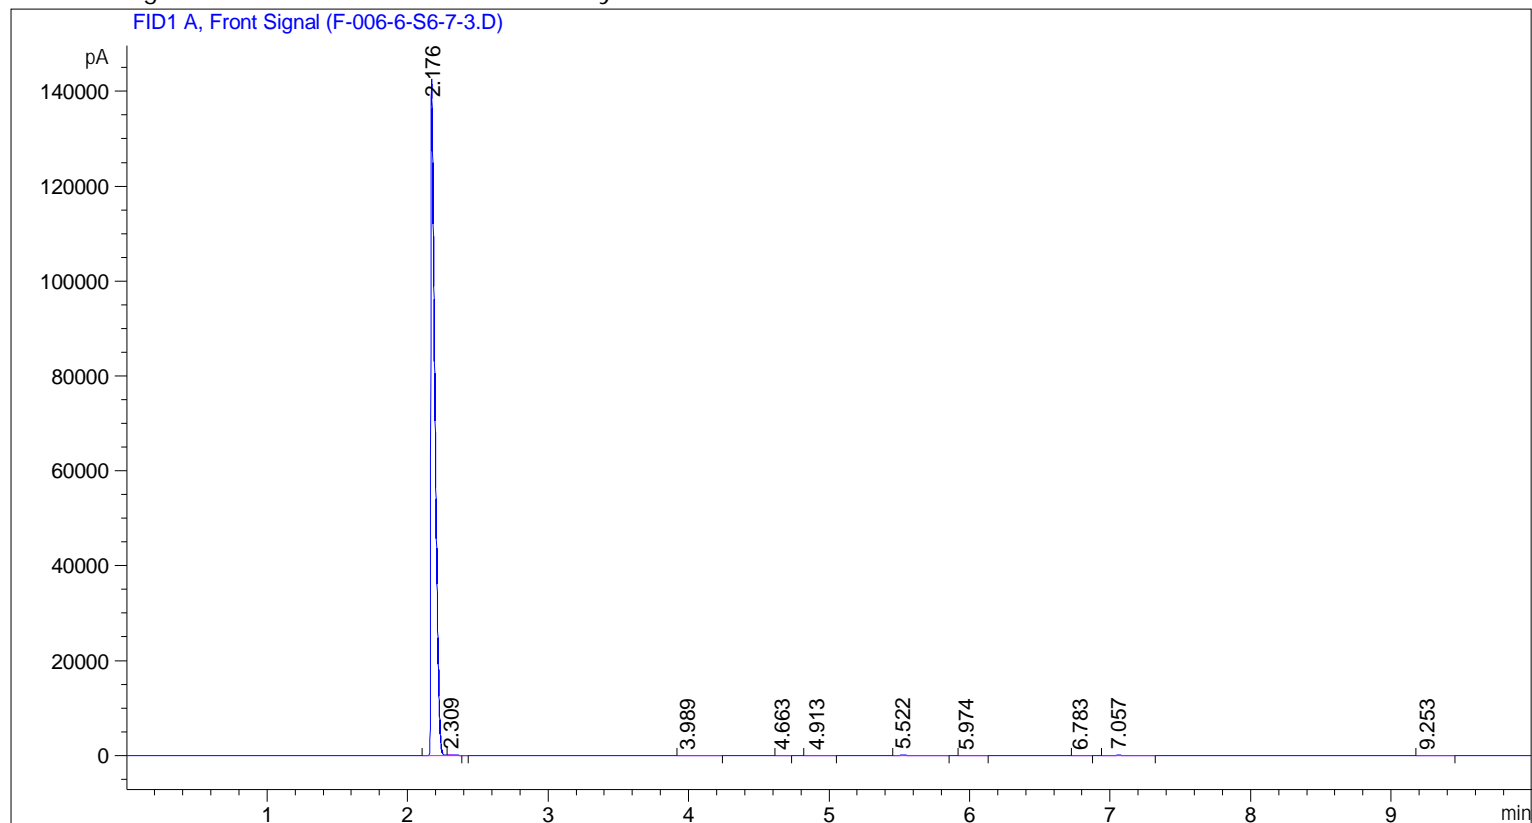

FID1 A, Front Signal (F-006-6-S6-7-3.D)

```
=====================================================================
                       Area Percent Report
=====================================================================


Sorted By             :       Signal
Calib. Data Modified  :       9/13/2021 3:53:03 PM
Multiplier            :       1.0000
Dilution              :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area      Area     Name
 #   [min]          [min]    [pA*s]       %
----|-------|------|-------|----------|--------|---------------------
  1   2.176 BB S    0.0308 2.86799e5  99.82925 ?
  2   2.309 BB T    0.0409  116.49449  0.04055 ?
  3   3.989 BB      0.0452   40.76227  0.01419 Acetate
  4   4.663 BB      0.0359    7.75798  0.00270 Propionate
  5   4.913 BB      0.0364    7.80751  0.00272 Isobutyrate
  6   5.522 BB      0.0356  194.39221  0.06766 Butyrate
  7   5.974 BB      0.0349    9.64633  0.00336 Isovaleric
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
8	6.783	BB	0.0353	8.01892	0.00279	Valeric
9	7.057	BB	0.0336	97.97503	0.03410	InternalSD
10	9.253	BB	0.0447	7.68648	0.00268	?

Totals :   2.87290e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

==
                       *** End of Report ***