


Sample Name: S4-1-1

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    5
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                     Location  :    5 (F)
Injection Date  : 3/20/2025 11:51:03 AM      Inj       :    1
                                           Inj Volume: 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-20 11-00-18
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
=====
```

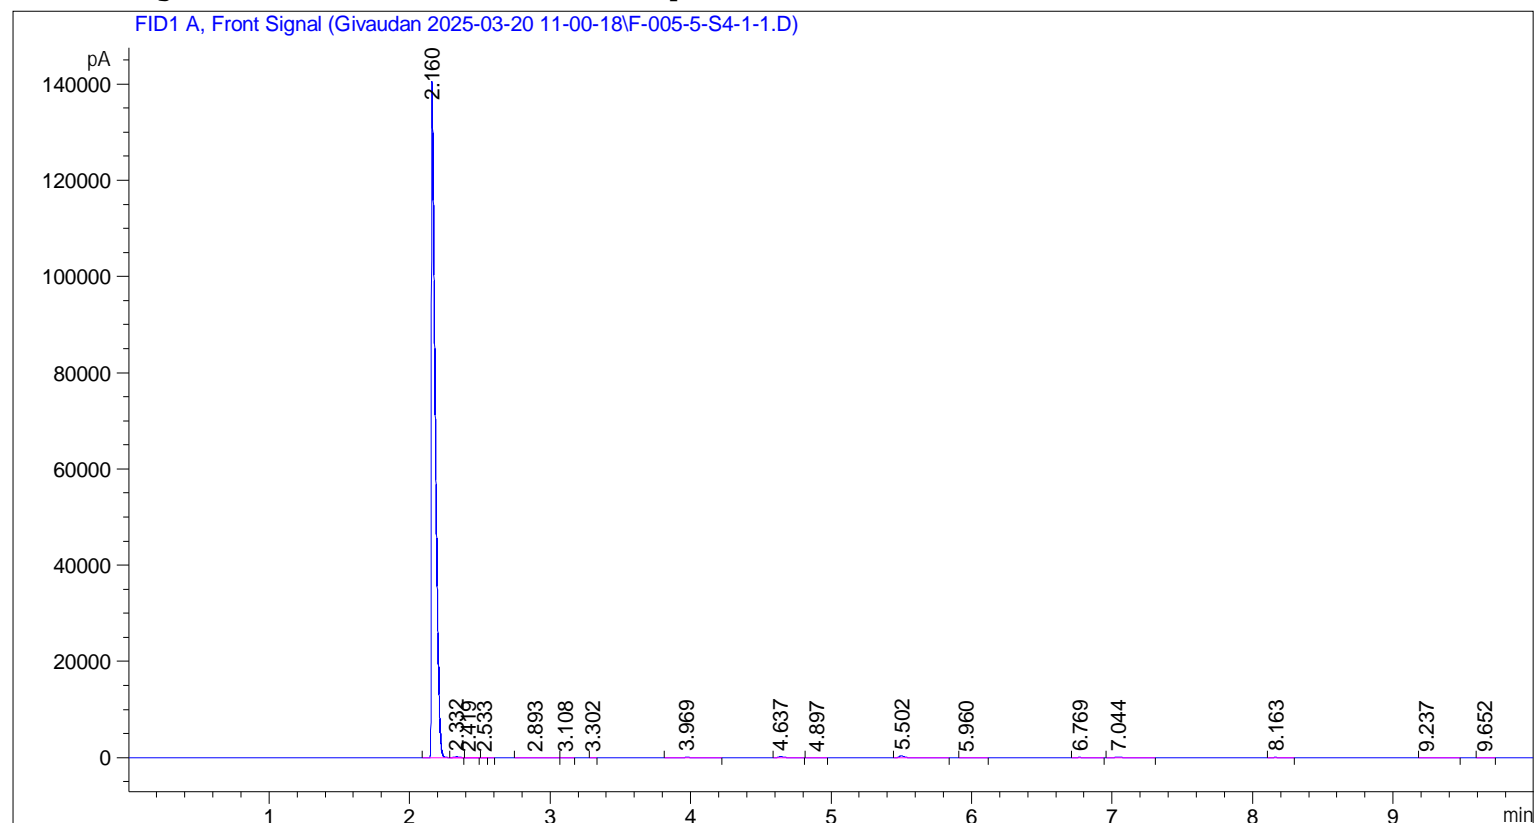

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.160	BB S	0.0275	2.62940e5	99.12719	?
2	2.332	BV T	0.0307	337.18738	0.12712	?
3	2.419	VV T	0.0498	13.45864	0.00507	?
4	2.533	VB T	0.0246	2.03027	0.00077	?
5	2.893	BB	0.0689	29.50526	0.01112	?
6	3.108	BB	0.0356	5.22798	0.00197	?
7	3.302	BB	0.0230	1.63320	0.00062	?
8	3.969	BB	0.0438	111.91421	0.04219	Acetate

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	4.637	BB	0.0339	493.87878	0.18619	Propionate
10	4.897	BB	0.0334	23.95386	0.00903	Isobutyrate
11	5.502	BB	0.0335	782.11127	0.29485	Butyrate
12	5.960	BB	0.0339	30.87564	0.01164	Isovaleric
13	6.769	BB	0.0334	68.67586	0.02589	Valeric
14	7.044	BB	0.0337	313.63269	0.11824	InternalSD
15	8.163	BB	0.0338	60.40704	0.02277	?
16	9.237	BB	0.0400	29.77103	0.01122	?
17	9.652	BB	0.0343	10.90569	0.00411	?

Totals : 2.65256e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====
*** End of Report ***