Data File C:\Users\P...hemStation\2\Data\Givaudan 2025-01-23 15-46-16\F-013-13-GD_P1_B12.D
Sample Name: GD_P1_B12

```
========================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   13
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   13   (F)
Injection Date  : 1/23/2025 6:03:50 PM                 Inj :    1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
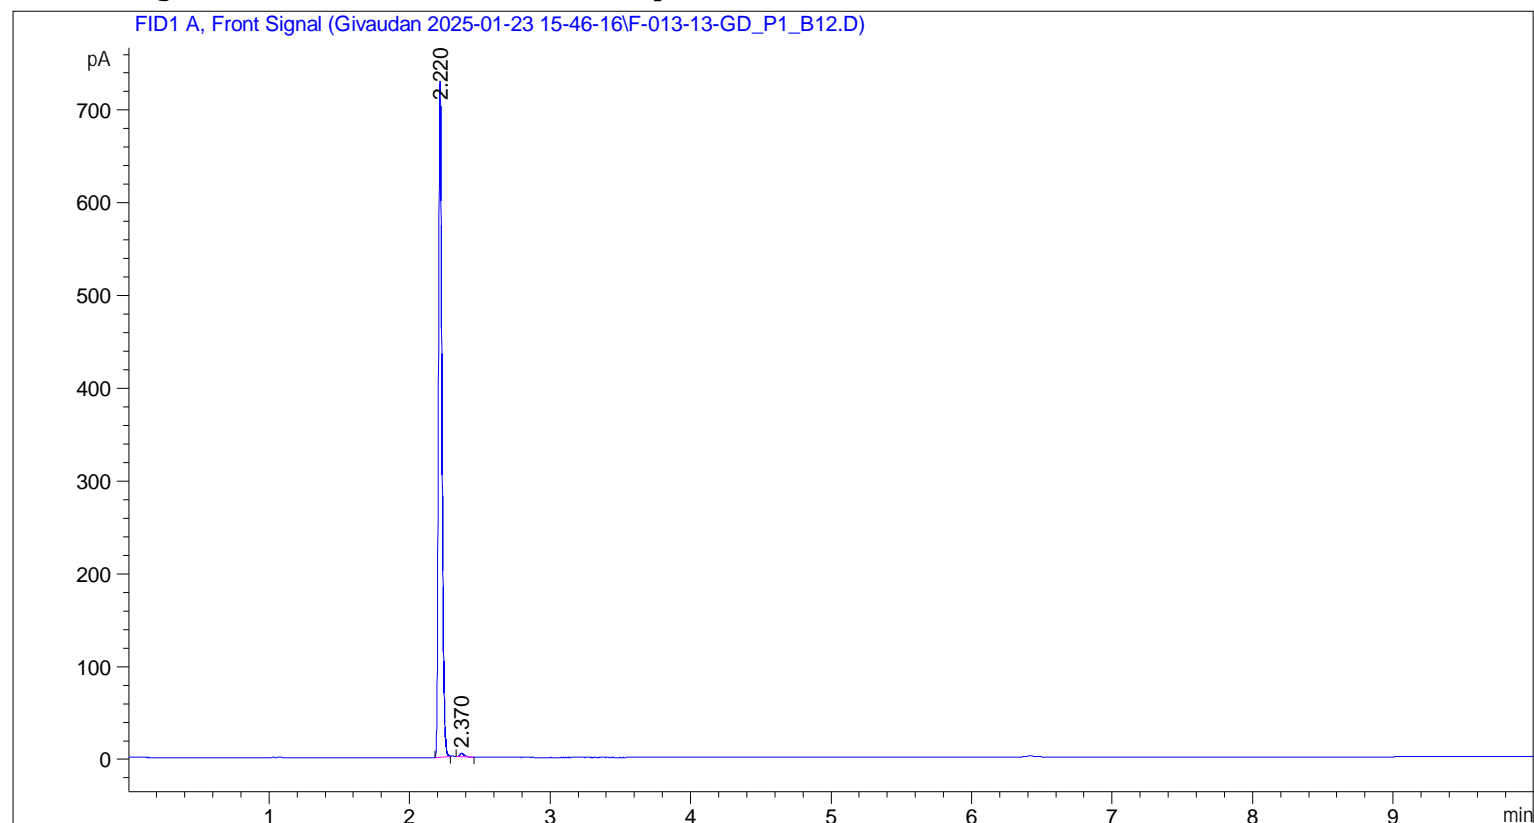

FID1 A, Front Signal (Givaudan 2025-01-23 15-46-16\F-013-13-GD_P1_B12.D)

```
========================================================================
                        Area Percent Report
========================================================================


Sorted By            :        Signal
Calib. Data Modified  :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]   [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
   1   2.220 BB      0.0270 1247.47644 99.29857 ?
   2   2.370 BB      0.0321    8.81194  0.70143 ?
   3   4.042         0.0000    0.00000  0.00000 Acetate
   4   4.725         0.0000    0.00000  0.00000 Propionate
   5   4.978         0.0000    0.00000  0.00000 Isobutyrate
   6   5.598         0.0000    0.00000  0.00000 Butyrate
   7   6.050         0.0000    0.00000  0.00000 Isovaleric
   8   6.869         0.0000    0.00000  0.00000 Valeric
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.139		0.0000	0.00000	0.00000	InternalSD

Totals :   1256.28838

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                          *** End of Report ***