Data File C:\Users\P...hemStation\2\Data\Givaudan 2025-01-22 12-09-16\F-013-13-GD_P1_A12.D
Sample Name: GD_P1_A12

```
====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   13
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   13   (F)
Injection Date  : 1/22/2025 2:30:45 PM              Inj :    1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
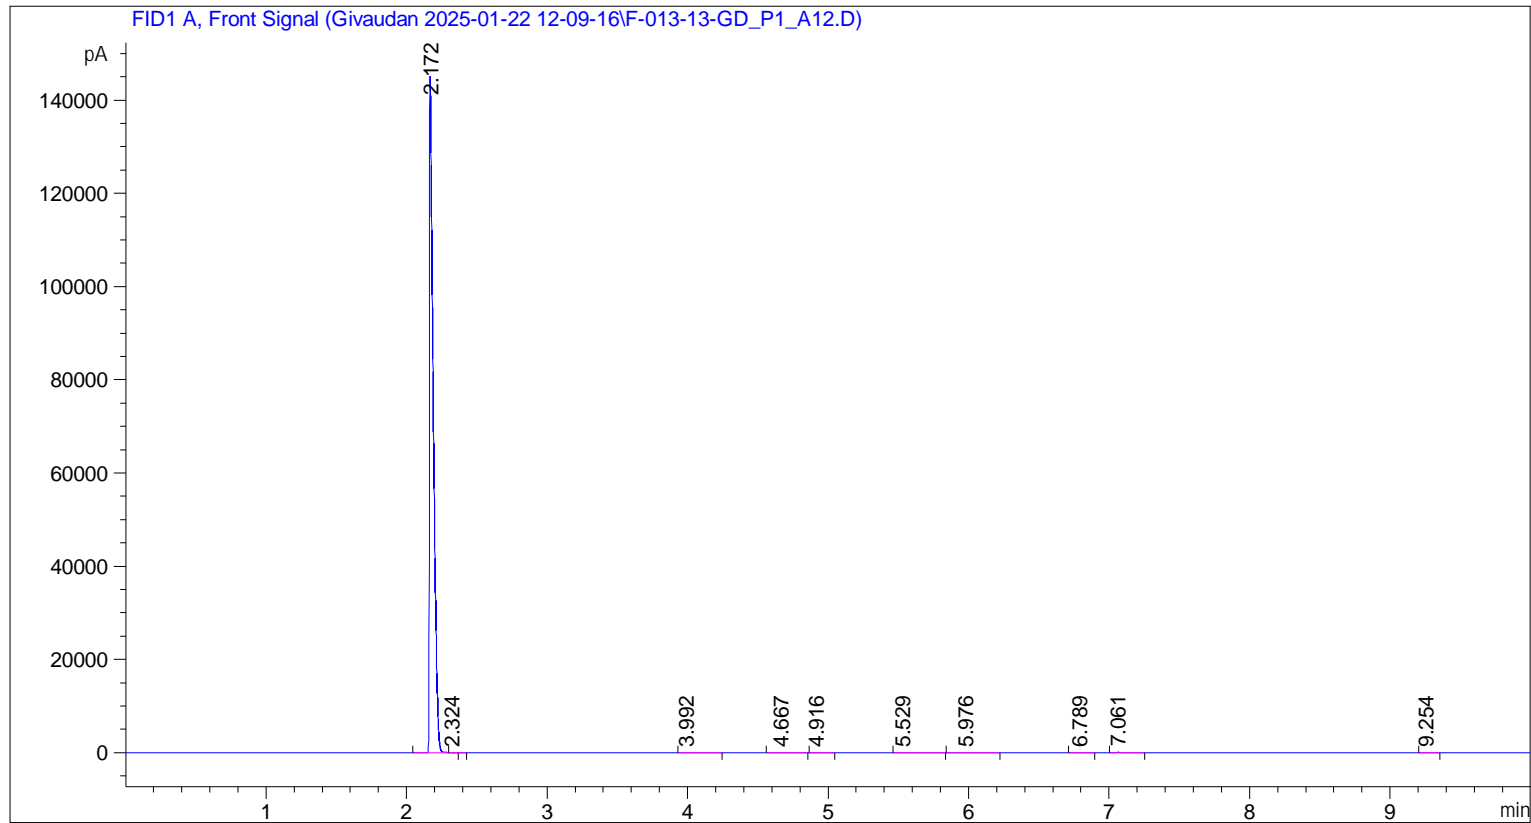

FID1 A, Front Signal (Givaudan 2025-01-22 12-09-16\F-013-13-GD_P1_A12.D)

```
====================================================================
                    Area Percent Report
====================================================================
```

```
Sorted By            :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier           :       1.0000
Dilution             :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.172	BB S	0.0289	2.77691e5	99.92673	?
2	2.324	BB T	0.0312	18.86324	0.00679	?
3	3.992	BB	0.0427	42.37632	0.01525	Acetate
4	4.667	BB	0.0370	19.86917	0.00715	Propionate
5	4.916	BB	0.0343	5.05245	0.00182	Isobutyrate
6	5.529	BB	0.0361	30.54668	0.01099	Butyrate
7	5.976	BB	0.0535	16.95972	0.00610	Isovaleric
8	6.789	BB	0.0366	5.58769	0.00201	Valeric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.061	BB	0.0347	60.27530	0.02169	InternalSD
10	9.254	BB	0.0370	4.06976	0.00146	?

Totals :   2.77895e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

==
                        *** End of Report ***