Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30\F-077-77-S2-16-3.D
Sample Name: S2-16-3

```
========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  77
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :  77  (F)
Injection Date  : 3/4/2025 1:48:18 AM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
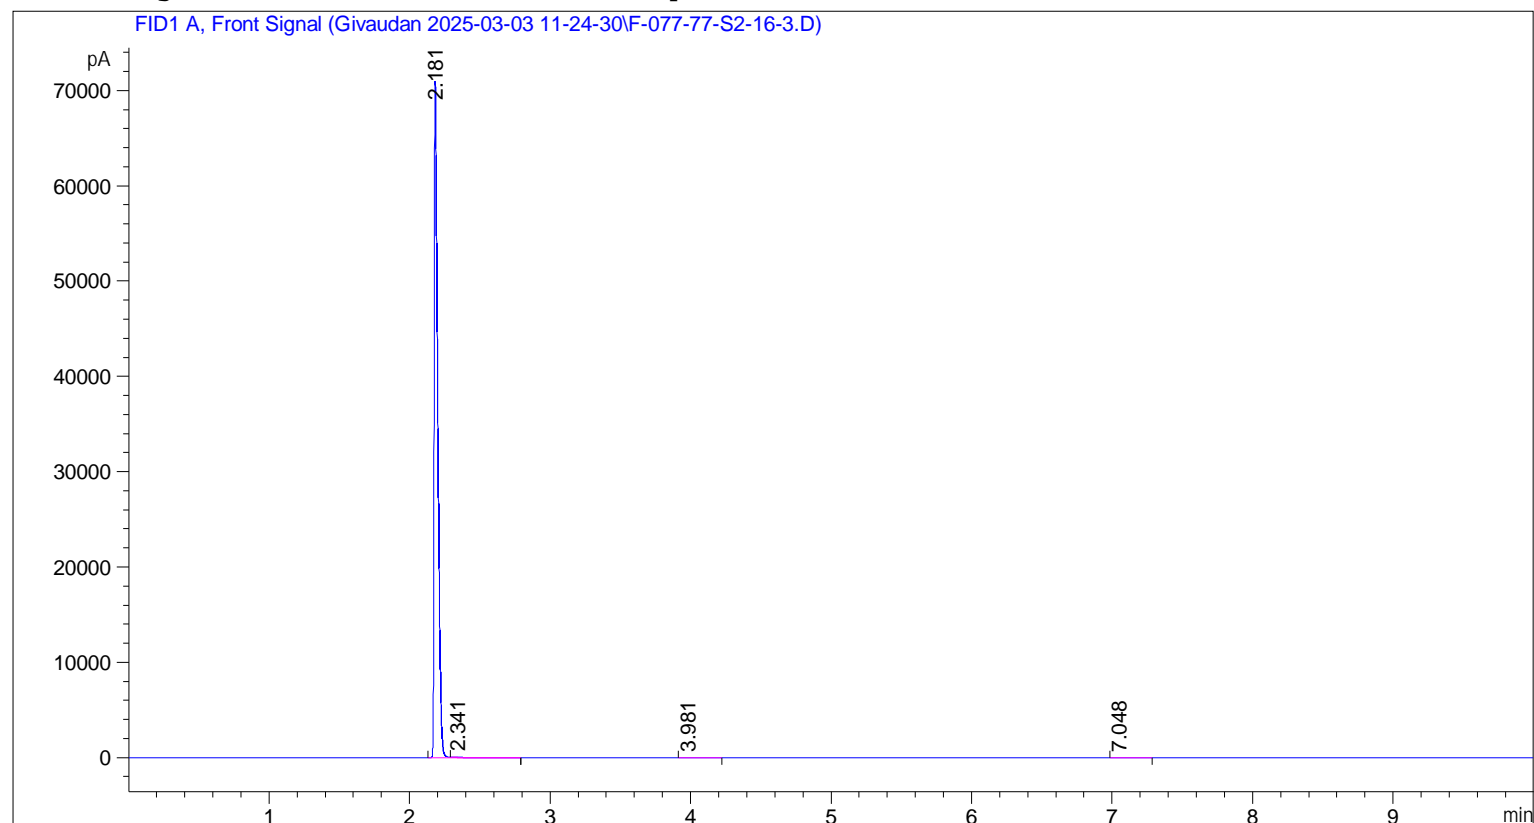

FID1 A, Front Signal (Givaudan 2025-03-03 11-24-30\F-077-77-S2-16-3.D)

```
========================================================================
                      Area Percent Report
========================================================================


Sorted By            :       Signal
Calib. Data Modified  :       9/13/2021 3:53:03 PM
Multiplier           :       1.0000
Dilution             :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area       Area      Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   2.181 BV R   0.0261 1.24884e5  99.90067 ?
   2   2.341 VB E   0.0639   91.05803  0.07284 ?
   3   3.981 BB     0.0457   11.02047  0.00882 Acetate
   4   4.725        0.0000    0.00000  0.00000 Propionate
   5   4.978        0.0000    0.00000  0.00000 Isobutyrate
   6   5.598        0.0000    0.00000  0.00000 Butyrate
   7   6.050        0.0000    0.00000  0.00000 Isovaleric
   8   6.869        0.0000    0.00000  0.00000 Valeric
```

```
  Peak RetTime  Type   Width     Area       Area     Name
   #   [min]           [min]    [pA*s]        %
 ----|-------|------|-------|----------|--------|--------------------
    9   7.048 BB      0.0384   22.09022  0.01767 InternalSD


 Totals :                     1.25008e5



 2 Warnings or Errors :

 Warning : Calibration warnings (see calibration table listing)
 Warning : Calibrated compound(s) not found

 =========================================================================
                          *** End of Report ***
```