Sample Name: D7

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   2
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   2   (F)
Injection Date  : 2/28/2025 1:43:53 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
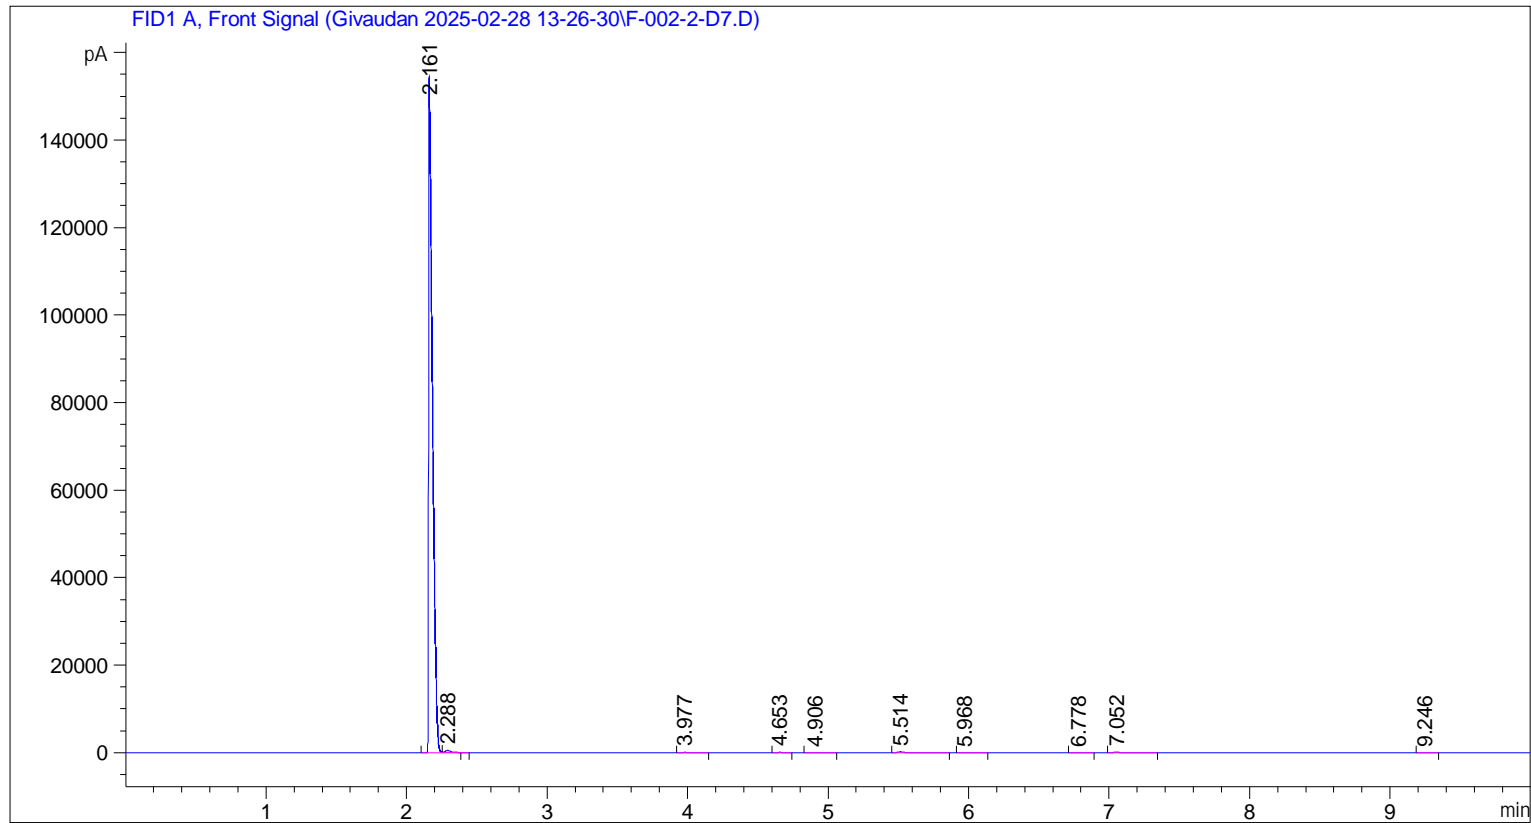

FID1 A, Front Signal (Givaudan 2025-02-28 13-26-30\F-002-2-D7.D)

```
=====================================================================
                       Area Percent Report
=====================================================================


Sorted By           :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier          :       1.0000
Dilution            :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]   [pA*s]          %
----|-------|------|-------|----------|--------|--------------------
   1   2.161 BB S    0.0282 2.92381e5  99.30302 ?
   2   2.288 BB T    0.0385 1266.38184  0.43011 ?
   3   3.977 BB      0.0376   75.23305  0.02555 Acetate
   4   4.653 BB      0.0340   74.86809  0.02543 Propionate
   5   4.906 BB      0.0341   14.17977  0.00482 Isobutyrate
   6   5.514 BB      0.0345  406.41357  0.13803 Butyrate
   7   5.968 BB      0.0345   18.87047  0.00641 Isovaleric
   8   6.778 BB      0.0351   17.02104  0.00578 Valeric
```

```
  Peak RetTime  Type   Width     Area       Area      Name
   #    [min]          [min]    [pA*s]       %
----|-------|------|-------|----------|--------|--------------------
    9   7.052 BB     0.0343  169.17506  0.05746 InternalSD
   10   9.246 BB     0.0374   10.00685  0.00340 ?


Totals :                     2.94434e5
```

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

```
=========================================================================
                        *** End of Report ***
```