Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16\F-002-2-GD_P1_A1.D
Sample Name: GD_P1_A1

```
========================================================================
Acq. Operator   : SYSTEM                         Seq. Line :   2
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                          Location :   2   (F)
Injection Date  : 1/22/2025 12:26:10 PM              Inj :   1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
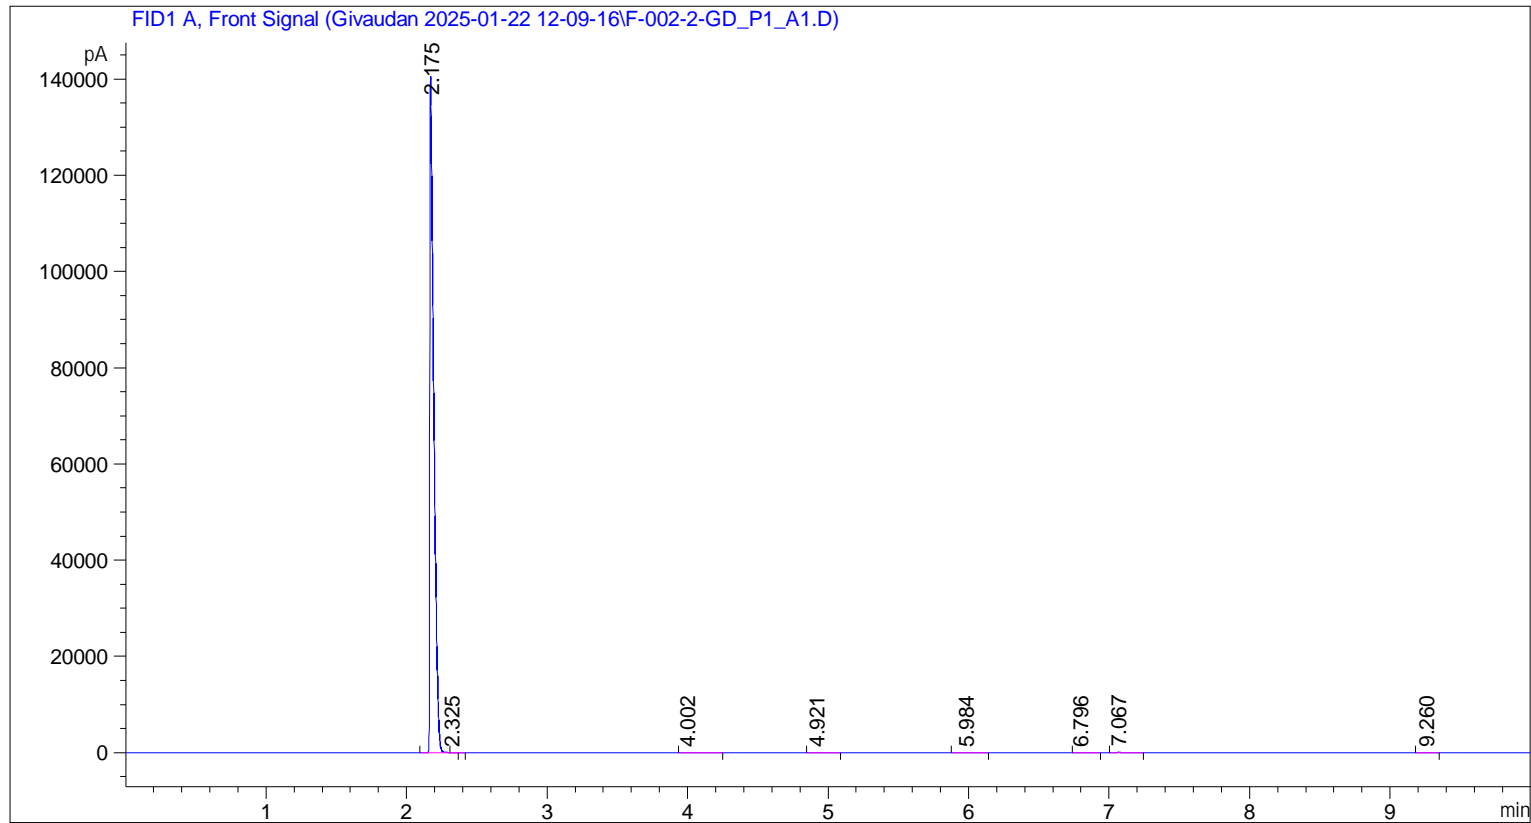

FID1 A, Front Signal (Givaudan 2025-01-22 12-09-16\F-002-2-GD_P1_A1.D)

```
========================================================================
                        Area Percent Report
========================================================================


Sorted By           :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier          :        1.0000
Dilution            :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]   [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
   1   2.175 BB S    0.0292 2.72978e5  99.95611 ?
   2   2.325 BB T    0.0319    7.22987  0.00265 ?
   3   4.002 BB      0.0487   21.89068  0.00802 Acetate
   4   4.725         0.0000    0.00000  0.00000 Propionate
   5   4.921 BB      0.0348    5.59318  0.00205 Isobutyrate
   6   5.598         0.0000    0.00000  0.00000 Butyrate
   7   5.984 BB      0.0352    6.78974  0.00249 Isovaleric
   8   6.796 BB      0.0382    6.14260  0.00225 Valeric
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.067	BB	0.0339	67.95209	0.02488	InternalSD
10	9.260	BB	0.0373	4.27285	0.00156	?

Totals :   2.73098e5

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                        *** End of Report ***