Data File C:\Users\P...ents\ChemStation\2\Data\Givaudan 2025-03-20 11-00-18\F-002-2-STD1.D
Sample Name: STD1

```
========================================================================
Acq. Operator   : SYSTEM                         Seq. Line :   2
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                          Location :   2  (F)
Injection Date  : 3/20/2025 11:17:04 AM               Inj :   1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-20 11-00-18
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
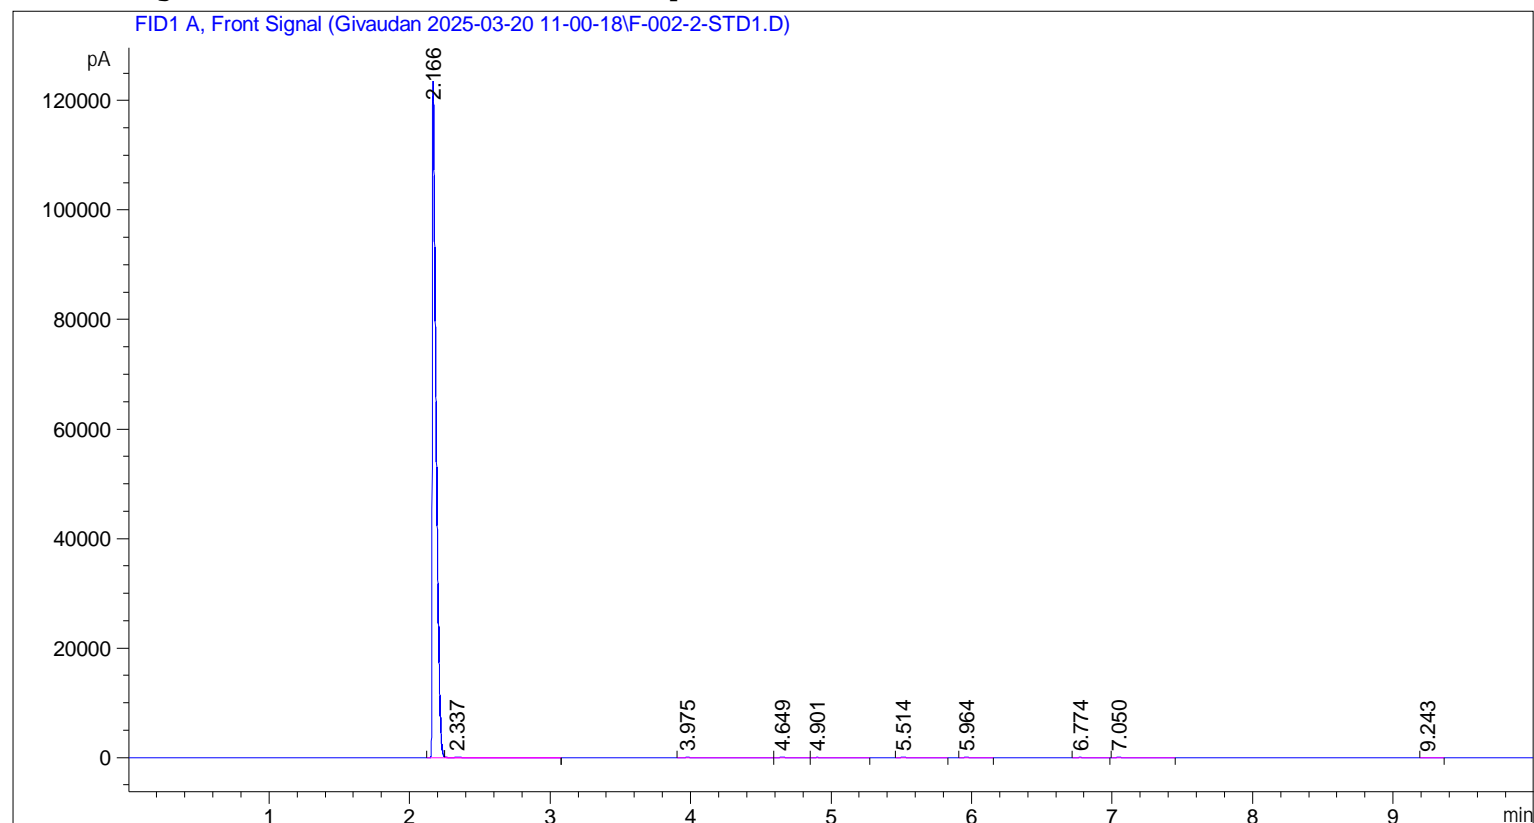


```
========================================================================
                        Area Percent Report
========================================================================


Sorted By            :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier           :       1.0000
Dilution             :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]   [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
   1   2.166 BV R    0.0276 2.28157e5   99.61351 ?
   2   2.337 VB E    0.0413  297.14923   0.12974 ?
   3   3.975 BV      0.0471   96.42336   0.04210 Acetate
   4   4.649 VV      0.0360  110.87332   0.04841 Propionate
   5   4.901 VB      0.0333   50.10711   0.02188 Isobutyrate
   6   5.514 BB      0.0338  104.75489   0.04574 Butyrate
   7   5.964 BB      0.0336   76.09653   0.03322 Isovaleric
   8   6.774 BB      0.0341   59.00198   0.02576 Valeric
```

Peak	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.050	BB	0.0331	86.74808	0.03787	InternalSD
10	9.243	BB	0.0390	4.07935	0.00178	?

Totals :   2.29042e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                          *** End of Report ***