```
=====================================================================
Acq. Operator   : SYSTEM                         Seq. Line :   7
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                          Location :   7  (F)
Injection Date  : 1/23/2025 4:55:55 PM                Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
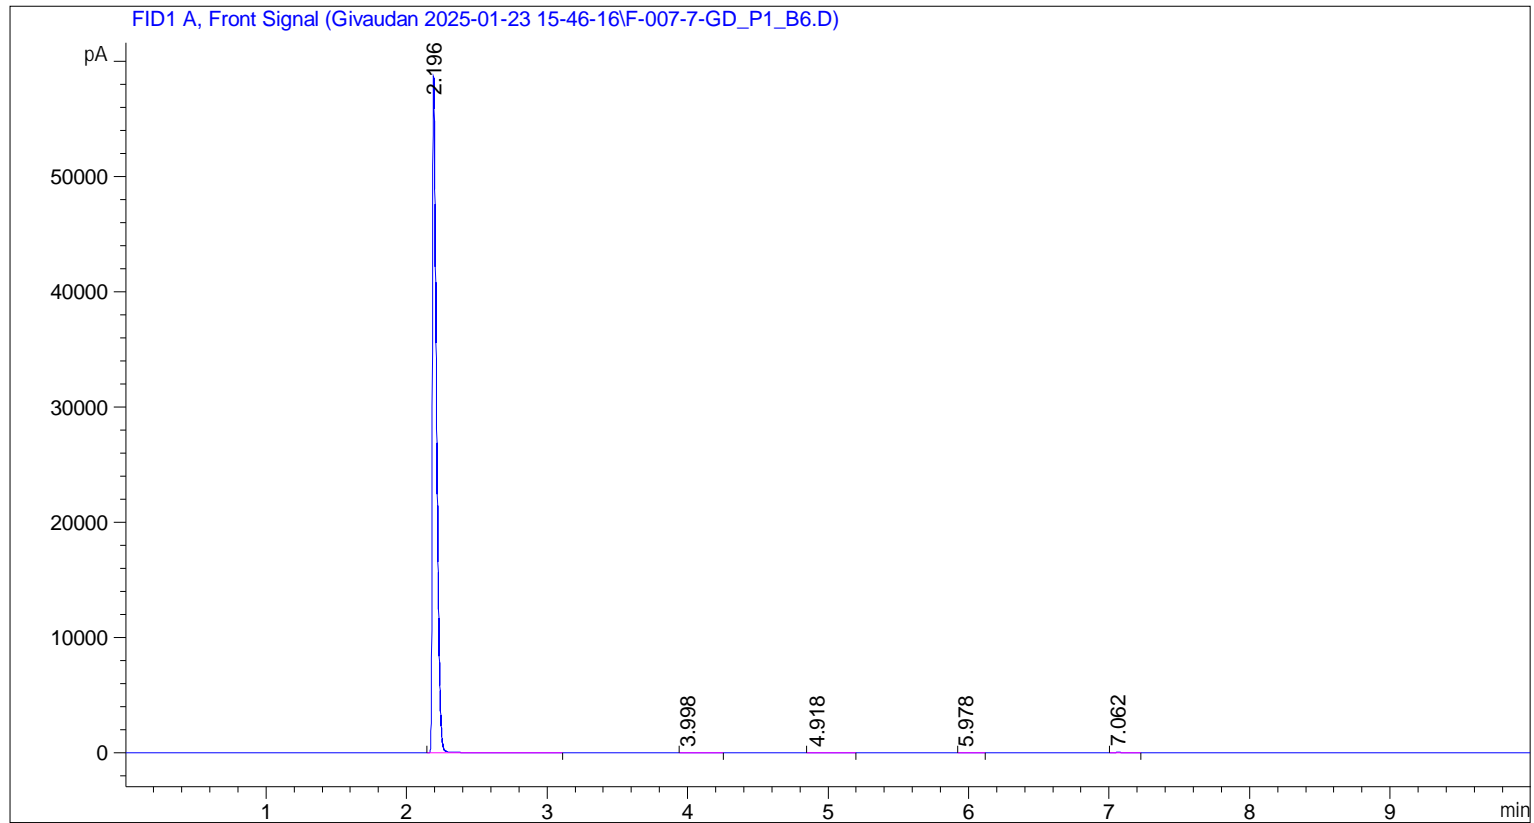

FID1 A, Front Signal (Givaudan 2025-01-23 15-46-16\F-007-7-GD_P1_B6.D)

```
=====================================================================
                       Area Percent Report
=====================================================================


Sorted By             :        Signal
Calib. Data Modified  :        9/13/2021 3:53:03 PM
Multiplier            :        1.0000
Dilution              :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal


Peak RetTime  Type   Width     Area       Area      Name
  #   [min]          [min]    [pA*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.196 BB      0.0297 1.18914e5  99.95094 ?
   2   3.998 BB      0.0443   11.37932  0.00956 Acetate
   3   4.725         0.0000    0.00000  0.00000 Propionate
   4   4.918 BB      0.0348    3.36040  0.00282 Isobutyrate
   5   5.598         0.0000    0.00000  0.00000 Butyrate
   6   5.978 BB      0.0343    3.78479  0.00318 Isovaleric
   7   6.869         0.0000    0.00000  0.00000 Valeric
   8   7.062 BB      0.0346   39.84803  0.03349 InternalSD
```

```
  Peak RetTime  Type   Width      Area        Area       Name
   #   [min]           [min]    [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
Totals :                      1.18972e5
```

  2 Warnings or Errors :

  Warning : Calibration warnings (see calibration table listing)
  Warning : Calibrated compound(s) not found

  ===
                        *** End of Report ***