Data File C:\Users\P...s\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30\F-078-78-S2-3-3.D
Sample Name: S2-3-3

```
=====================================================================
Acq. Operator   : SYSTEM                         Seq. Line :  78
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                          Location :  78  (F)
Injection Date  : 3/4/2025 1:59:38 AM                 Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
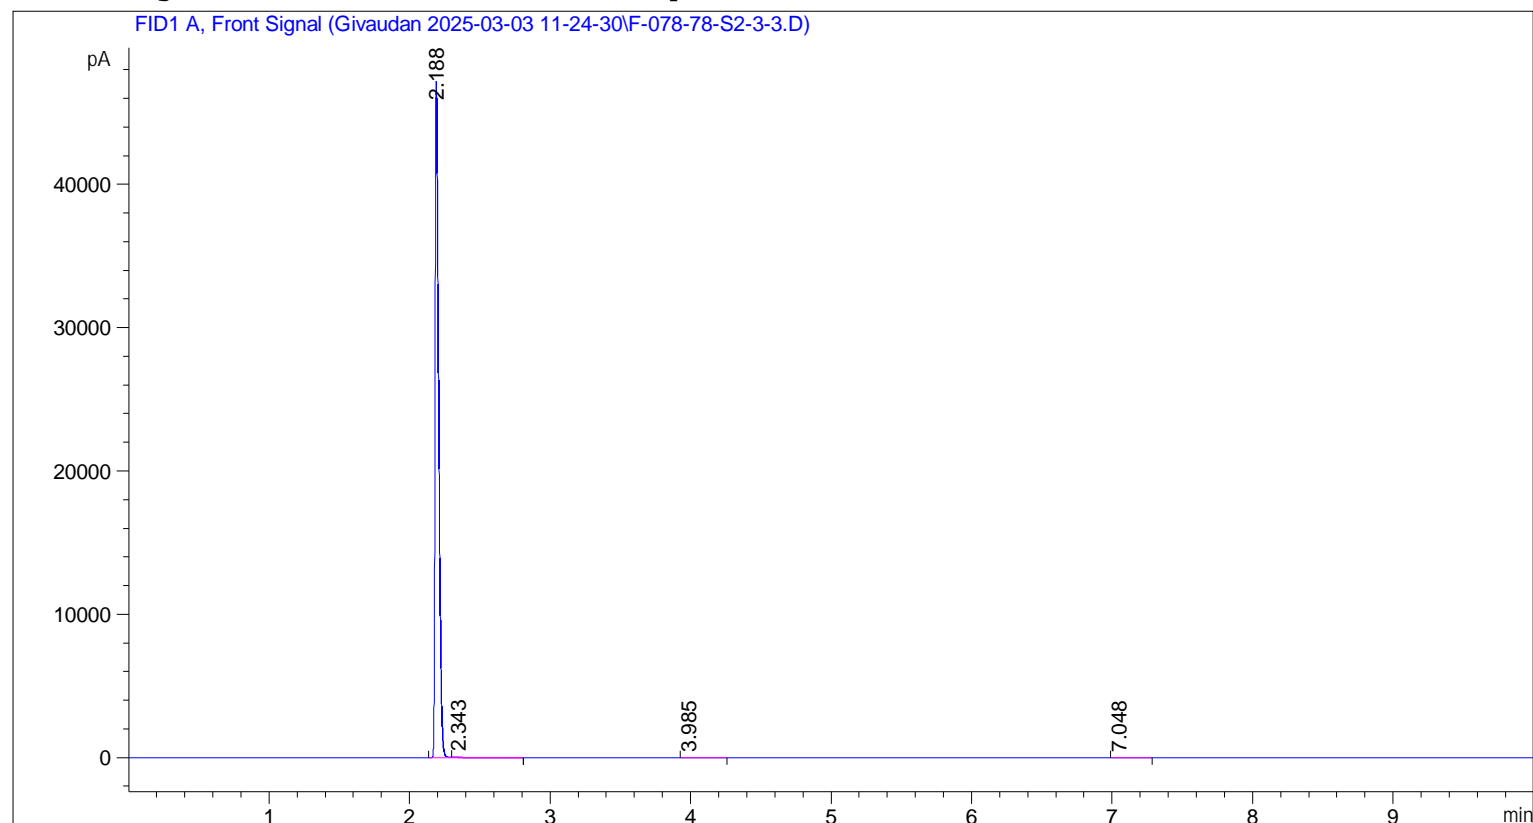

FID1 A, Front Signal (Givaudan 2025-03-03 11-24-30\F-078-78-S2-3-3.D)

```
=====================================================================
                        Area Percent Report
=====================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   2.188 BV R    0.0270 8.29987e4  99.91527 ?
   2   2.343 VB E    0.0779   47.29459  0.05693 ?
   3   3.985 BB      0.0480    8.10651  0.00976 Acetate
   4   4.725         0.0000    0.00000  0.00000 Propionate
   5   4.978         0.0000    0.00000  0.00000 Isobutyrate
   6   5.598         0.0000    0.00000  0.00000 Butyrate
   7   6.050         0.0000    0.00000  0.00000 Isovaleric
   8   6.869         0.0000    0.00000  0.00000 Valeric
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.048	BB	0.0381	14.98284	0.01804	InternalSD

Totals :   8.30691e4

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                          *** End of Report ***