Data File C:\Users\P...ments\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30\F-015-15-E8.D
Sample Name: E8

```
==================================================================
Acq. Operator   : SYSTEM                      Seq. Line :  15
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                       Location :  15  (F)
Injection Date  : 2/28/2025 4:11:08 PM             Inj :   1
                                              Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
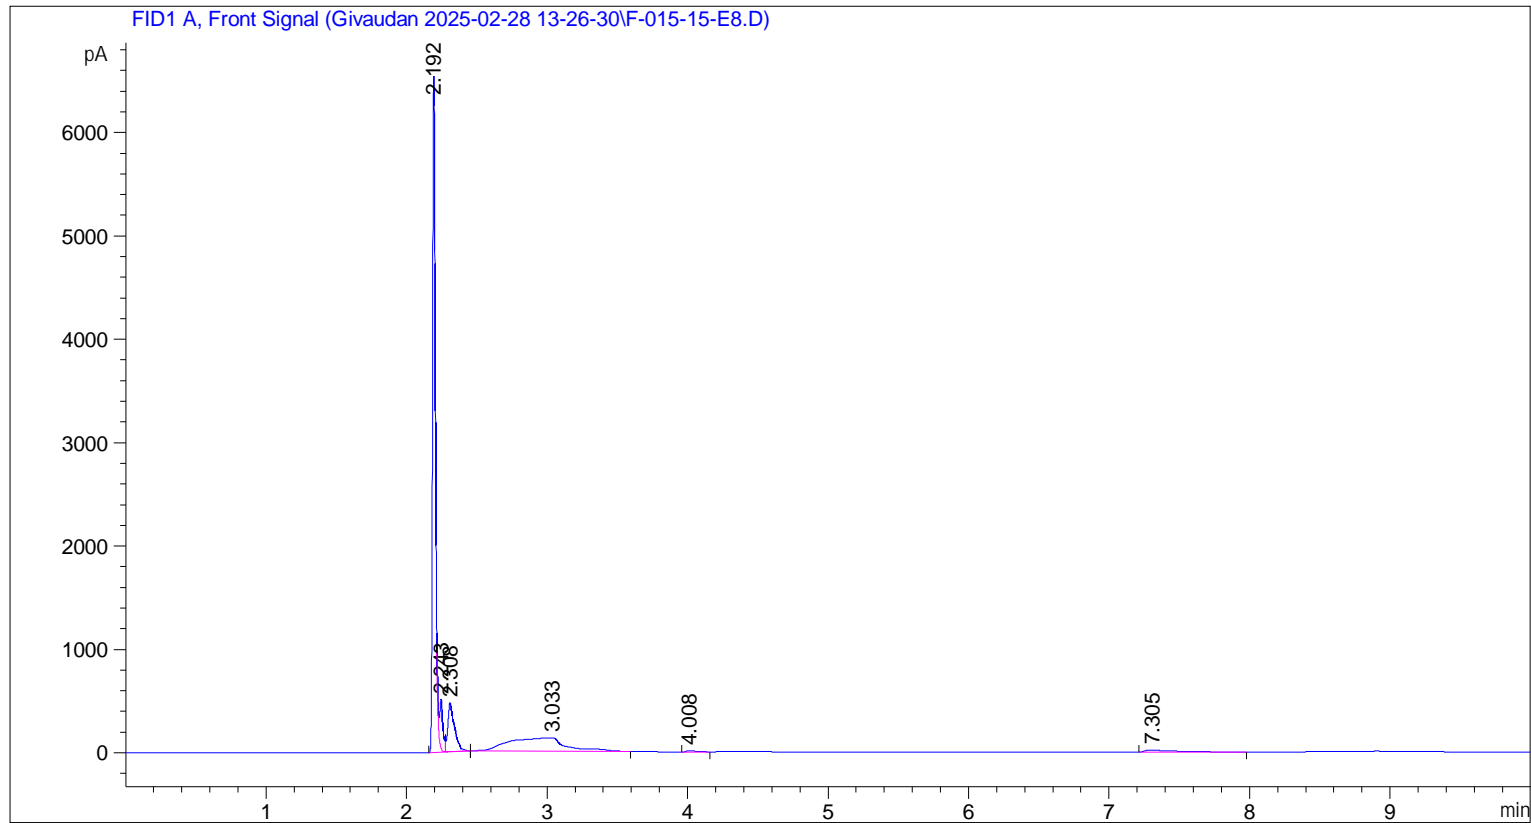

FID1 A, Front Signal (Givaudan 2025-02-28 13-26-30\F-015-15-E8.D)

```
==================================================================
                    Area Percent Report
==================================================================

Sorted By             :      Signal
Calib. Data Modified  :      9/13/2021 3:53:03 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

```
Peak RetTime  Type   Width     Area       Area      Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
  1   2.192 BV R    0.0217 9444.11426 59.89624 ?
  2   2.243 VV E    0.0229  748.74469  4.74867 ?
  3   2.308 VB E    0.0455 1545.71033  9.80317 ?
  4   3.033 BB      0.3482 3694.72070 23.43257 ?
  5   4.008 BB      0.0758   54.60970  0.34634 Acetate
  6   4.725         0.0000    0.00000  0.00000 Propionate
  7   4.978         0.0000    0.00000  0.00000 Isobutyrate
  8   5.598         0.0000    0.00000  0.00000 Butyrate
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	6.050		0.0000	0.00000	0.00000	Isovaleric
10	6.869		0.0000	0.00000	0.00000	Valeric
11	7.305	BB	0.2131	279.55673	1.77300	InternalSD

Totals :   1.57675e4

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                          *** End of Report ***