Data File C:\Users\P...ments\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30\F-013-13-E6.D
Sample Name: E6

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  13
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   13  (F)
Injection Date  : 2/28/2025 3:48:27 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
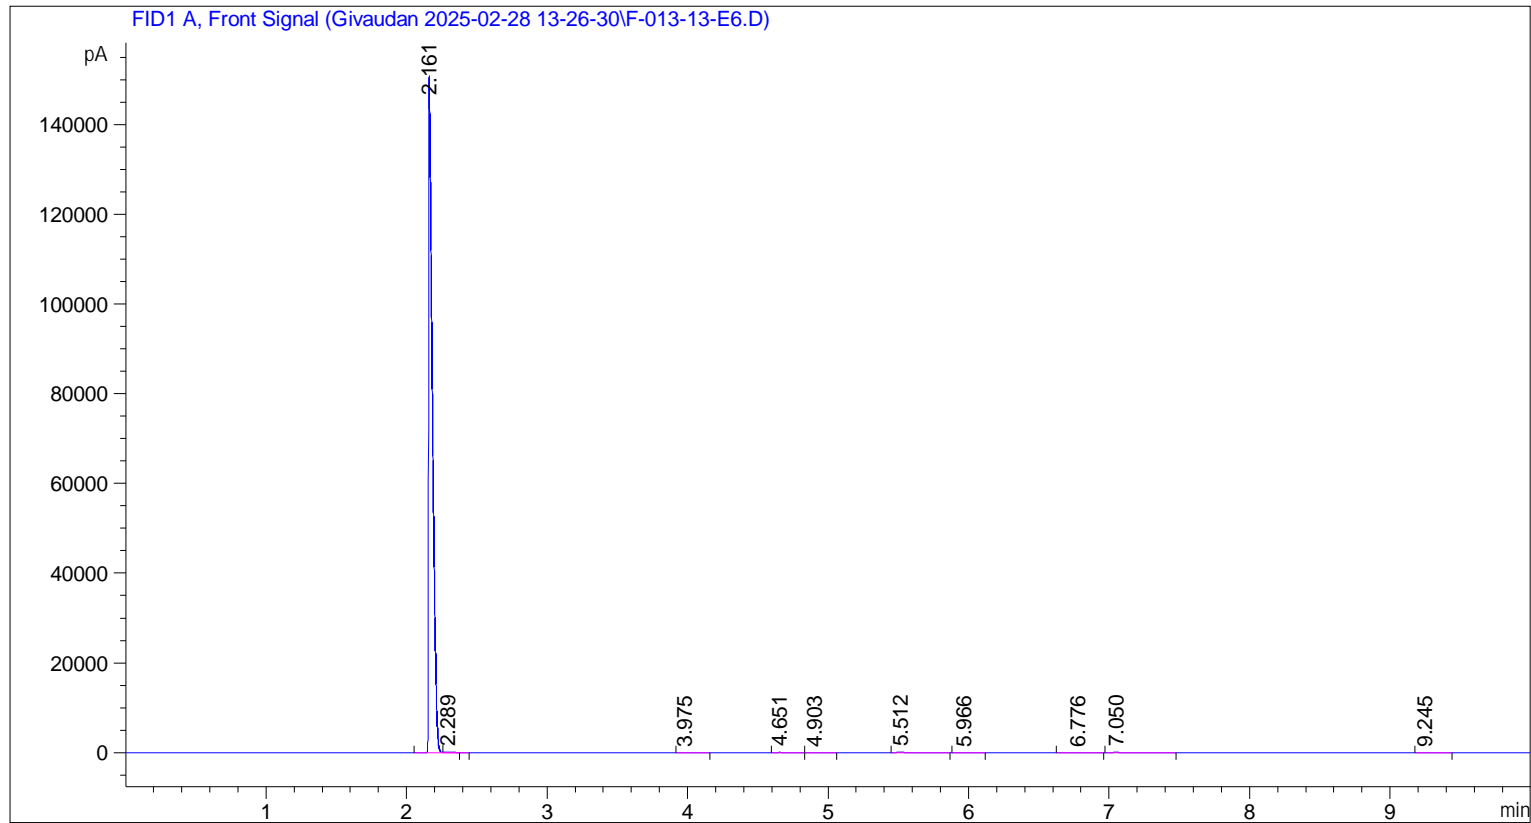

FID1 A, Front Signal (Givaudan 2025-02-28 13-26-30\F-013-13-E6.D)

```
=====================================================================
                        Area Percent Report
=====================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.161	BB S	0.0271	2.81446e5	99.69055	?
2	2.289	BB T	0.0390	288.64868	0.10224	?
3	3.975	BB	0.0378	52.27725	0.01852	Acetate
4	4.651	BB	0.0353	66.45949	0.02354	Propionate
5	4.903	BB	0.0339	10.27741	0.00364	Isobutyrate
6	5.512	BB	0.0346	305.43152	0.10819	Butyrate
7	5.966	BB	0.0357	13.88482	0.00492	Isovaleric
8	6.776	BB	0.0386	14.06125	0.00498	Valeric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.050	BB	0.0346	112.77154	0.03994	InternalSD
10	9.245	BB	0.0486	9.83471	0.00348	?

Totals :   2.82320e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                        *** End of Report ***