Data File C:\Users\P...ChemStation\2\Data\Givaudan 2025-01-23 15-46-16\F-010-10-GD_P1_B9.D
Sample Name: GD_P1_B9

```
========================================================================
Acq. Operator   : SYSTEM                         Seq. Line :  10
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                          Location :  10  (F)
Injection Date  : 1/23/2025 5:29:54 PM                Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
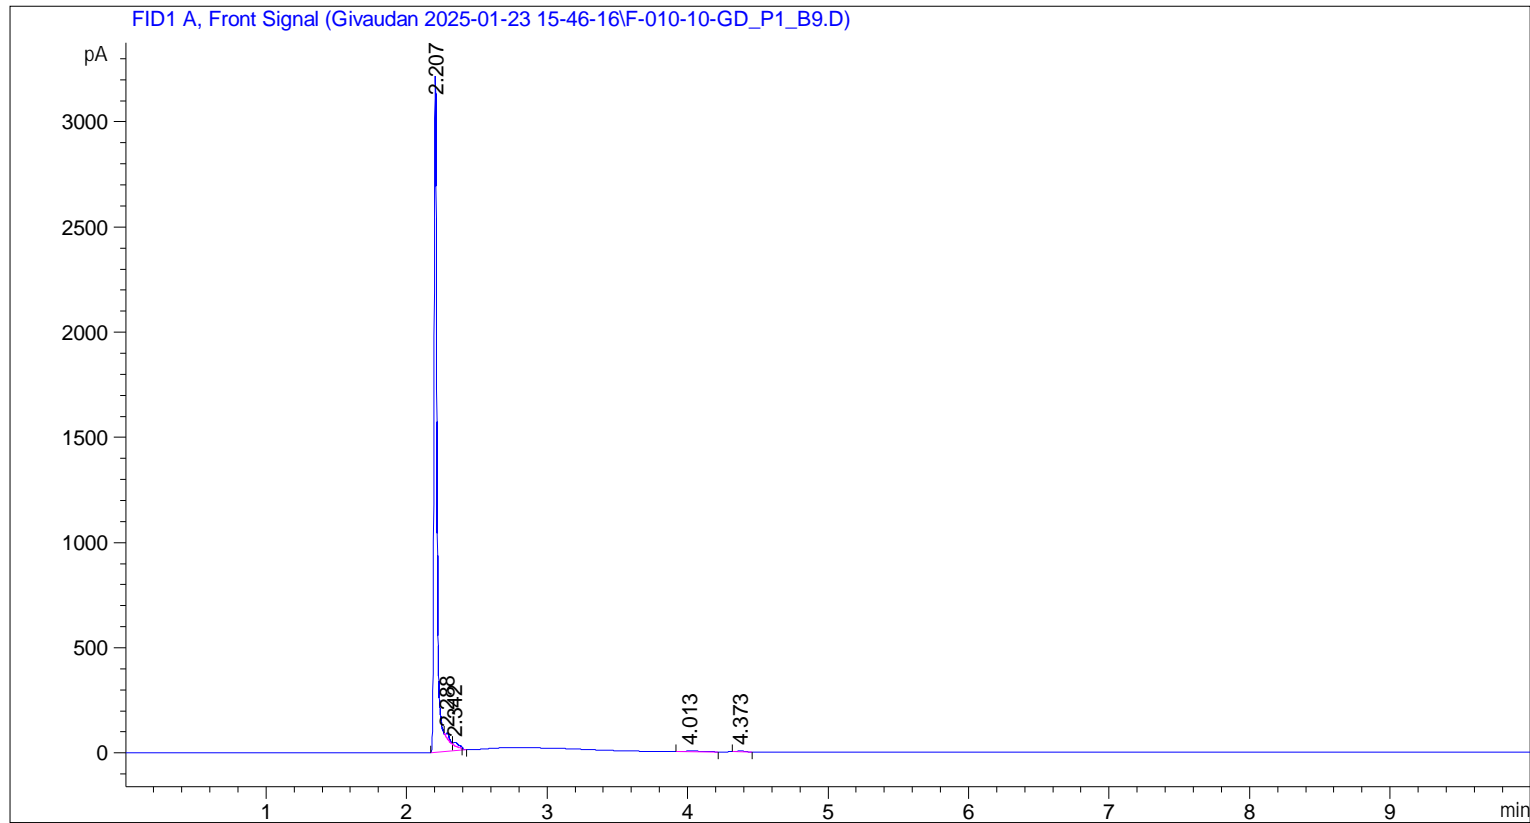

FID1 A, Front Signal (Givaudan 2025-01-23 15-46-16\F-010-10-GD_P1_B9.D)

```
========================================================================
                        Area Percent Report
========================================================================


Sorted By            :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier           :       1.0000
Dilution             :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]    [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
   1   2.207 BV R    0.0240 4891.60400 97.47159 ?
   2   2.288 VV E    0.0229   36.65615  0.73042 ?
   3   2.342 VB E    0.0447   46.68274  0.93021 ?
   4   4.013 BB      0.0782   26.72829  0.53260 Acetate
   5   4.373 BB      0.0526   16.82071  0.33517 ?
   6   4.725         0.0000    0.00000  0.00000 Propionate
   7   4.978         0.0000    0.00000  0.00000 Isobutyrate
   8   5.598         0.0000    0.00000  0.00000 Butyrate
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	6.050		0.0000	0.00000	0.00000	Isovaleric
10	6.869		0.0000	0.00000	0.00000	Valeric
11	7.139		0.0000	0.00000	0.00000	InternalSD

Totals :   5018.49190

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                        *** End of Report ***