```
========================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   10
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   10  (F)
Injection Date  : 4/16/2025 4:58:23 PM              Inj :    1
                                              Inj Volume : 1 µl
Sequence File   : C:\Users\Public\Documents\ChemStation\2\Data\std 2025-04-16 15-15-06\std.S
Method          : C:\Users\Public\Documents\ChemStation\2\Data\std 2025-04-16 15-15-06\SCFA_
                  FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
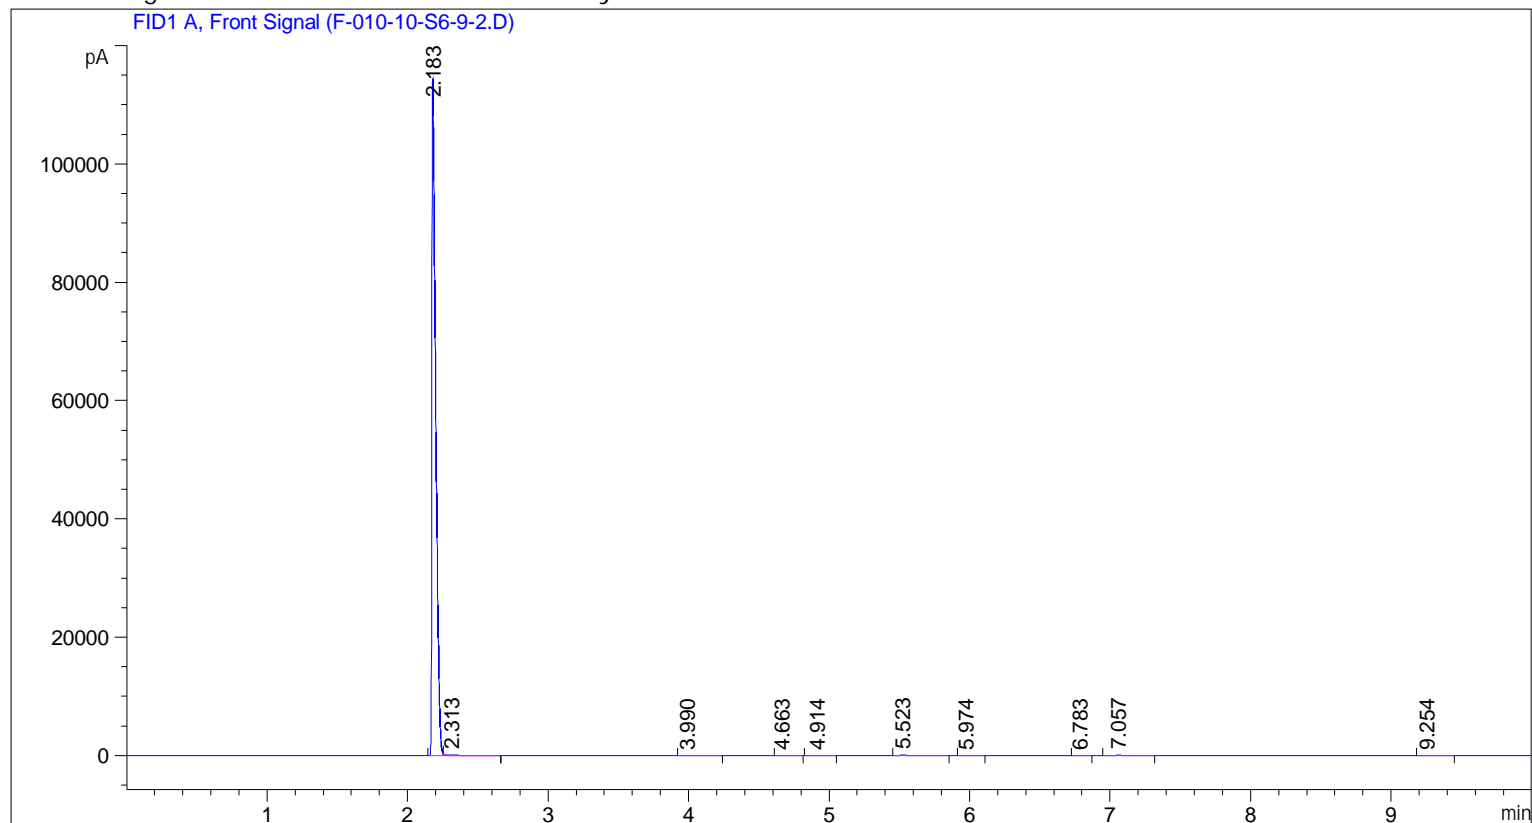

FID1 A, Front Signal (F-010-10-S6-9-2.D)

```
========================================================================
                        Area Percent Report
========================================================================
```

```
Sorted By            :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier           :       1.0000
Dilution             :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

```
Peak RetTime  Type   Width     Area      Area      Name
 #   [min]          [min]    [pA*s]       %
----|-------|-------|-------|----------|--------|--------------------
  1   2.183 BV R    0.0278 2.14979e5  99.73348 ?
  2   2.313 VB E    0.0666   275.49448  0.12781 ?
  3   3.990 BB      0.0445    39.87822  0.01850 Acetate
  4   4.663 BB      0.0360    17.10684  0.00794 Propionate
  5   4.914 BB      0.0348     6.69404  0.00311 Isobutyrate
  6   5.523 BB      0.0344   131.41835  0.06097 Butyrate
  7   5.974 BB      0.0354     8.24267  0.00382 Isovaleric
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
8	6.783	BB	0.0350	6.69249	0.00310	Valeric
9	7.057	BB	0.0343	82.10995	0.03809	InternalSD
10	9.254	BB	0.0449	6.86269	0.00318	?

Totals :   2.15554e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                        *** End of Report ***