


```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    1
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                     Location  :    1 (F)
Injection Date  : 3/20/2025 11:05:45 AM      Inj       :    1
                                           Inj Volume: 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-20 11-00-18
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
=====
```

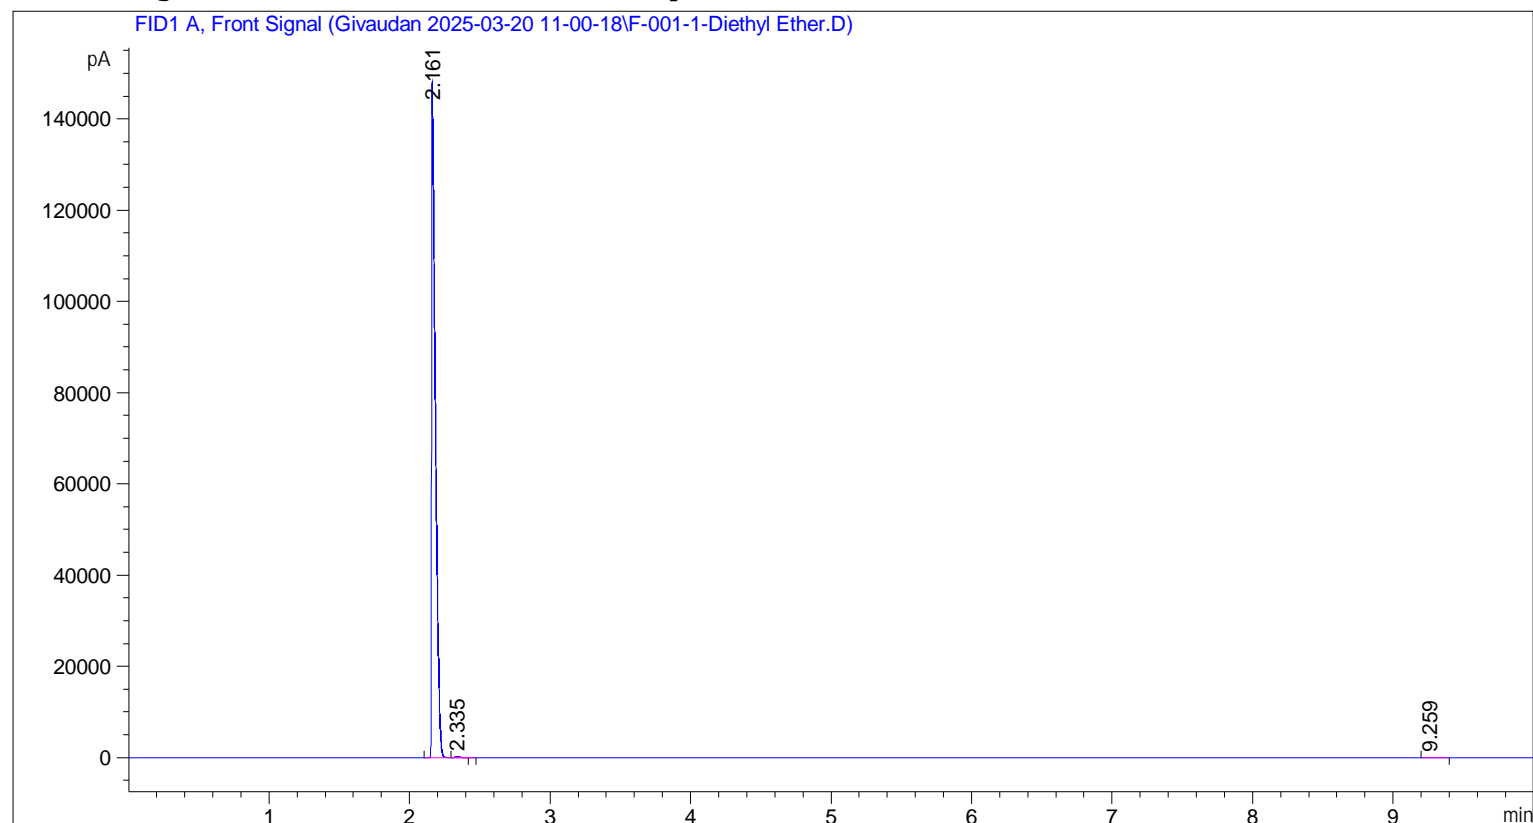

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.161	BB S	0.0270	2.74950e5	99.78943	?
2	2.335	BB T	0.0300	563.85138	0.20464	?
3	4.042		0.0000	0.00000	0.00000	Acetate
4	4.725		0.0000	0.00000	0.00000	Propionate
5	4.978		0.0000	0.00000	0.00000	Isobutyrate
6	5.598		0.0000	0.00000	0.00000	Butyrate
7	6.050		0.0000	0.00000	0.00000	Isovaleric
8	6.869		0.0000	0.00000	0.00000	Valeric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.139		0.0000	0.00000	0.00000	InternalSD
10	9.259	BB	0.0380	16.34373	0.00593	?

Totals : 2.75531e5

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*