


```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    3
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                     Location  :    3 (F)
Injection Date  : 2/28/2025 11:25:10 AM      Inj       :    1
                                           Inj Volume: 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-28 10-58-58
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
=====
```

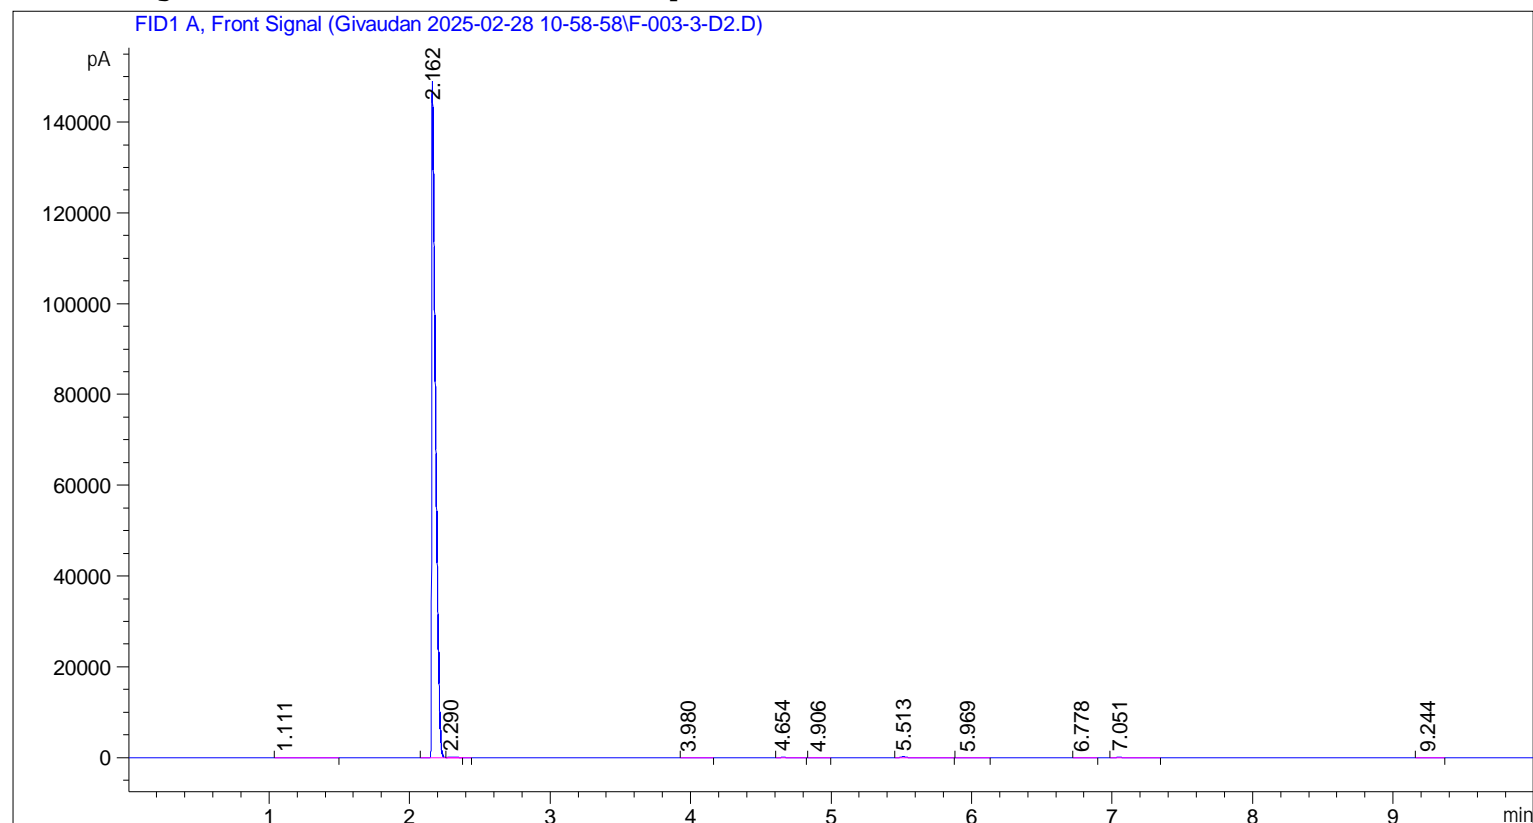

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.111	BB	0.0521	17.91619	0.00643	?
2	2.162	BB S	0.0277	2.77488e5	99.57515	?
3	2.290	BB T	0.0387	353.97235	0.12702	?
4	3.980	BB	0.0390	57.71252	0.02071	Acetate
5	4.654	BB	0.0359	106.71449	0.03829	Propionate
6	4.906	BB	0.0338	12.06269	0.00433	Isobutyrate
7	5.513	BB	0.0343	463.24966	0.16623	Butyrate
8	5.969	BB	0.0354	16.28073	0.00584	Isovaleric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	6.778	BB	0.0358	14.83054	0.00532	Valeric
10	7.051	BB	0.0341	132.45386	0.04753	InternalSD
11	9.244	BB	0.0404	8.74286	0.00314	?

Totals : 2.78672e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====
*** End of Report ***