Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16\F-005-5-GD_P1_B4.D
Sample Name: GD_P1_B4

```
========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   5
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   5  (F)
Injection Date  : 1/23/2025 4:33:16 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
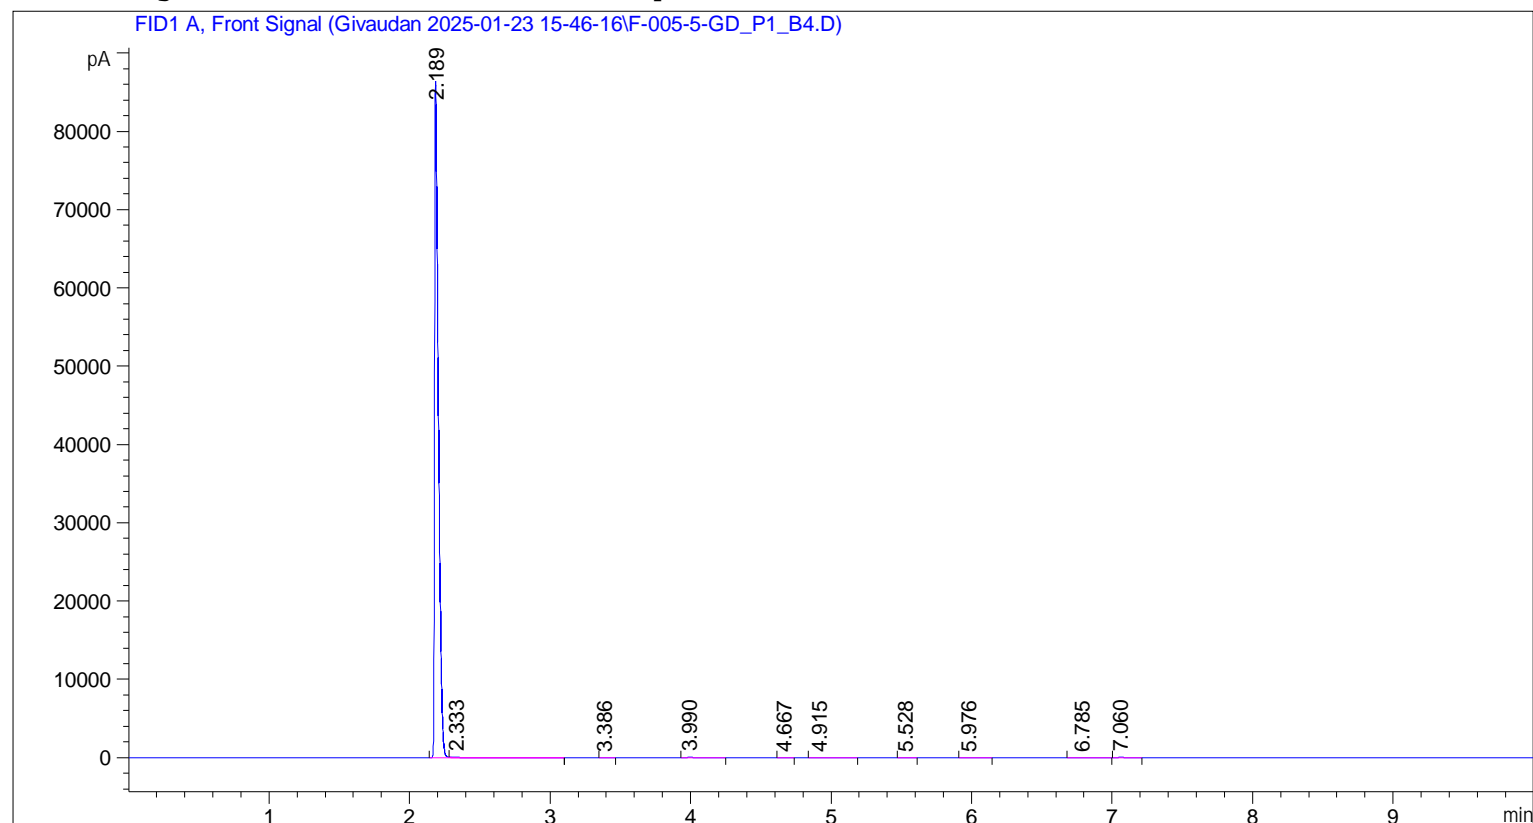

FID1 A, Front Signal (Givaudan 2025-01-23 15-46-16\F-005-5-GD_P1_B4.D)

```
========================================================================
                        Area Percent Report
========================================================================


Sorted By           :       Signal
Calib. Data Modified :       9/13/2021 3:53:03 PM
Multiplier          :       1.0000
Dilution            :       1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area       Area     Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   2.189 BV R    0.0279 1.60659e5  99.77555 ?
   2   2.333 VB E    0.0809  133.40370  0.08285 ?
   3   3.386 BB      0.0280    2.33527  0.00145 ?
   4   3.990 BB      0.0387   75.73598  0.04704 Acetate
   5   4.667 BB      0.0331    2.97024  0.00184 Propionate
   6   4.915 BB      0.0322   22.23837  0.01381 Isobutyrate
   7   5.528 BB      0.0339    8.94430  0.00555 Butyrate
   8   5.976 BB      0.0329   27.47620  0.01706 Isovaleric
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	6.785	BB	0.0350	26.27637	0.01632	Valeric
10	7.060	BB	0.0328	62.02143	0.03852	InternalSD

Totals :   1.61020e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

==
                          *** End of Report ***