Data File C:\Users\P...hemStation\2\Data\Givaudan 2025-01-22 12-09-16\F-012-12-GD_P1_A11.D
Sample Name: GD_P1_A11

```
========================================================================
Acq. Operator   : SYSTEM                        Seq. Line :  12
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :  12  (F)
Injection Date  : 1/22/2025 2:19:25 PM                Inj :   1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
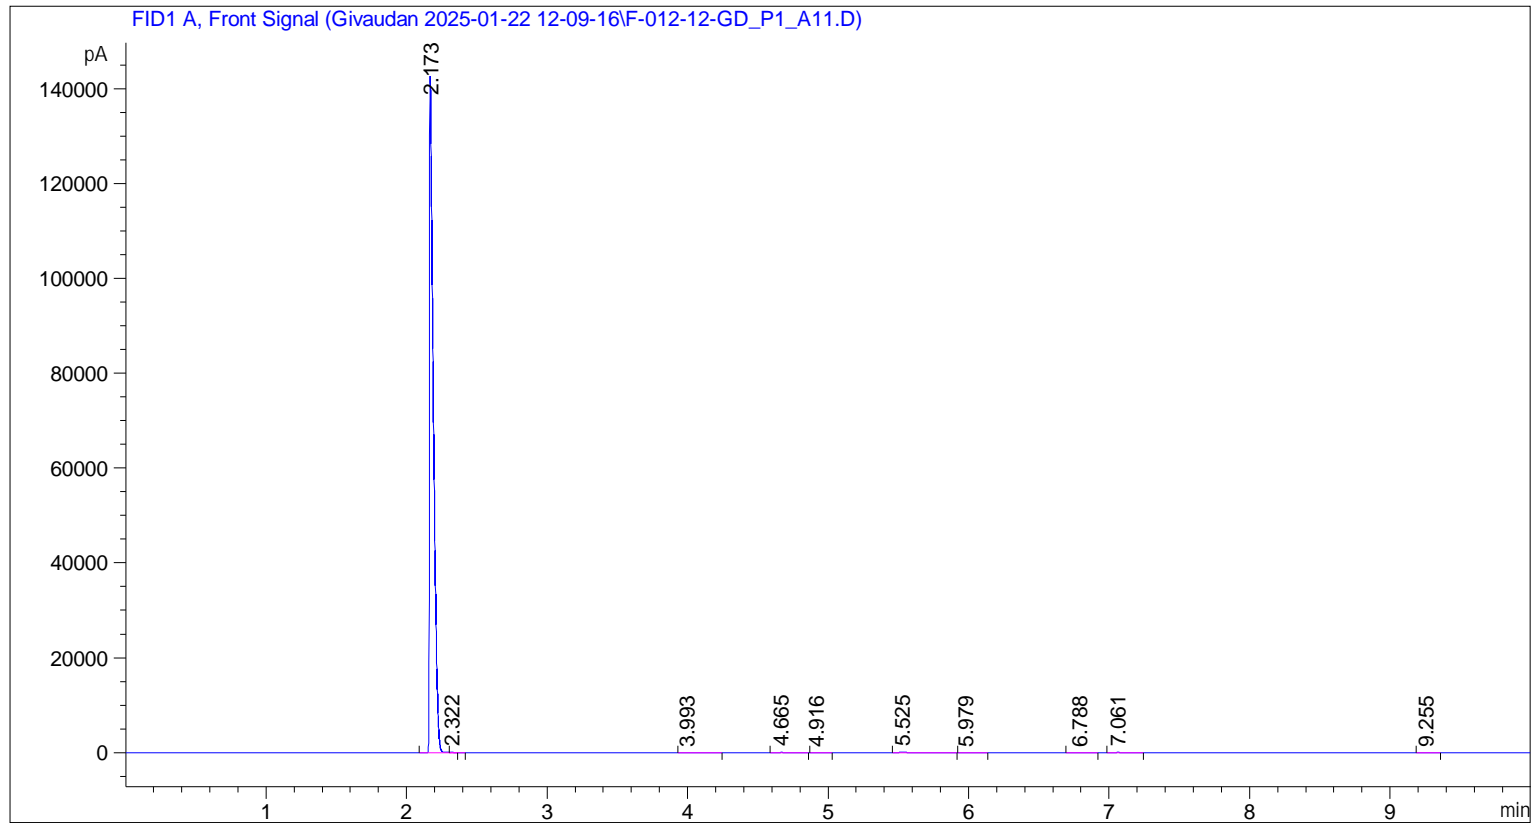

FID1 A, Front Signal (Givaudan 2025-01-22 12-09-16\F-012-12-GD_P1_A11.D)

```
========================================================================
                        Area Percent Report
========================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.173	BB S	0.0289	2.75575e5	99.83030	?
2	2.322	BB T	0.0314	14.89094	0.00539	?
3	3.993	BB	0.0432	28.40326	0.01029	Acetate
4	4.665	BB	0.0365	65.41229	0.02370	Propionate
5	4.916	BB	0.0340	6.15047	0.00223	Isobutyrate
6	5.525	BB	0.0358	268.27567	0.09719	Butyrate
7	5.979	BB	0.0366	9.14685	0.00331	Isovaleric
8	6.788	BB	0.0368	8.14508	0.00295	Valeric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.061	BB	0.0338	63.97231	0.02317	InternalSD
10	9.255	BB	0.0386	4.05785	0.00147	?

Totals :   2.76044e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                          *** End of Report ***