Data File C:\Users\P...ChemStation\2\Data\Givaudan 2025-01-22 12-09-16\F-010-10-GD_P1_A9.D
Sample Name: GD_P1_A9

```
========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  10
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :  10  (F)
Injection Date  : 1/22/2025 1:56:46 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
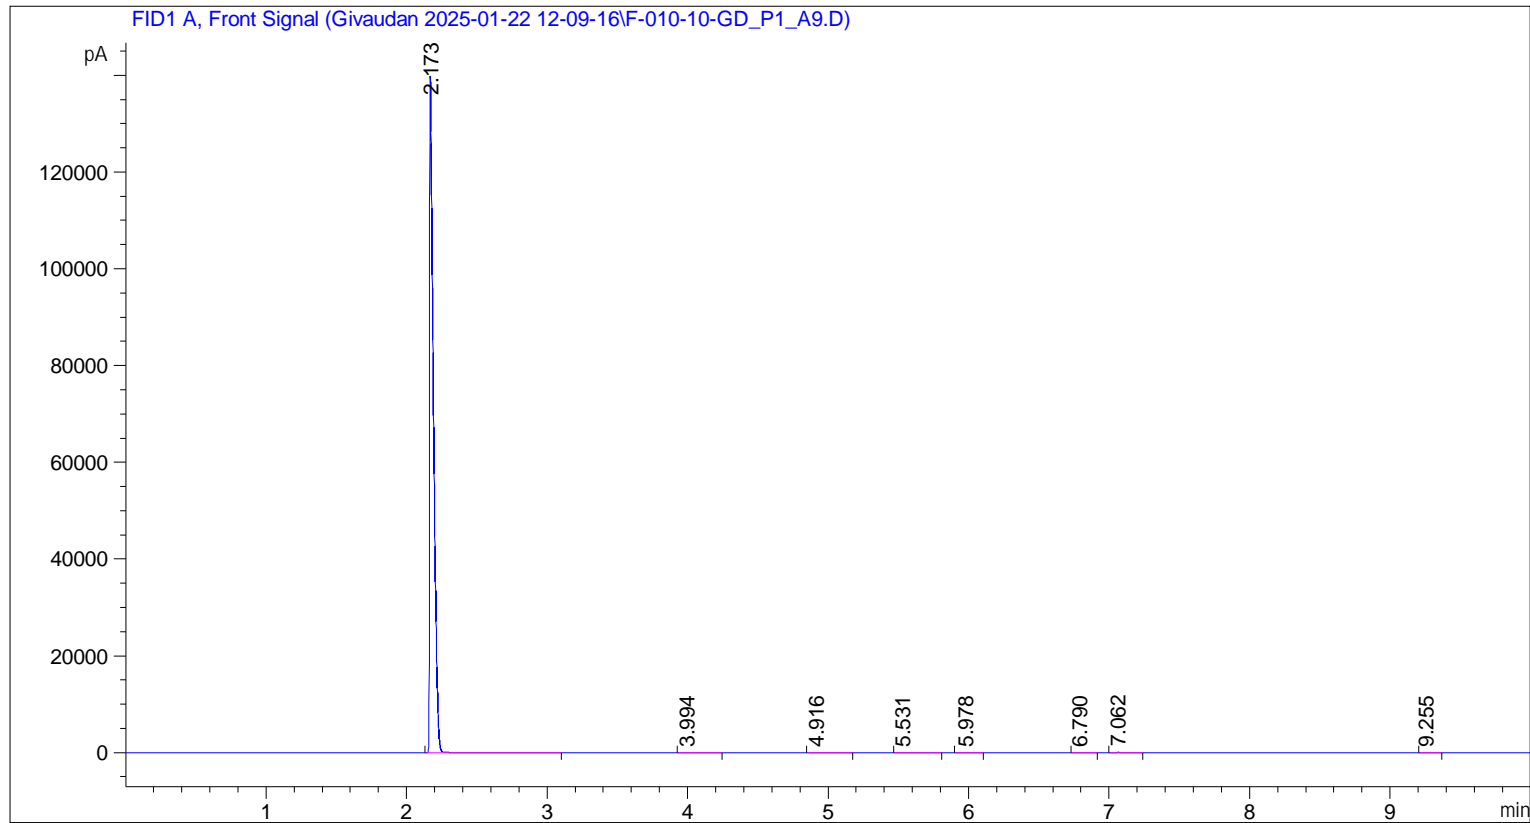

FID1 A, Front Signal (Givaudan 2025-01-22 12-09-16\F-010-10-GD_P1_A9.D)

```
========================================================================
                        Area Percent Report
========================================================================


Sorted By             :        Signal
Calib. Data Modified  :        9/13/2021 3:53:03 PM
Multiplier            :        1.0000
Dilution              :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area      Name
  #   [min]          [min]   [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
   1   2.173 BB      0.0272 2.67089e5   99.95599 ?
   2   3.994 BB      0.0444   36.22924   0.01356 Acetate
   3   4.725         0.0000    0.00000   0.00000 Propionate
   4   4.916 BB      0.0343    4.15617   0.00156 Isobutyrate
   5   5.531 BB      0.0361    5.41115   0.00203 Butyrate
   6   5.978 BB      0.0353    4.77497   0.00179 Isovaleric
   7   6.790 BB      0.0372    4.42410   0.00166 Valeric
   8   7.062 BB      0.0346   58.70845   0.02197 InternalSD
```

```
   Peak RetTime  Type   Width     Area       Area      Name
    #    [min]          [min]   [pA*s]        %
  ----|-------|------|-------|----------|--------|--------------------
     9   9.255 BB     0.0375    3.89570  0.00146 ?


   Totals :                     2.67206e5



   2 Warnings or Errors :

   Warning : Calibration warnings (see calibration table listing)
   Warning : Calibrated compound(s) not found

   =======================================================================
                         *** End of Report ***
```