Data File C:\Users\P...ents\ChemStation\2\Data\Givaudan 2025-03-20 11-00-18\F-006-6-STD2.D
Sample Name: STD2

===
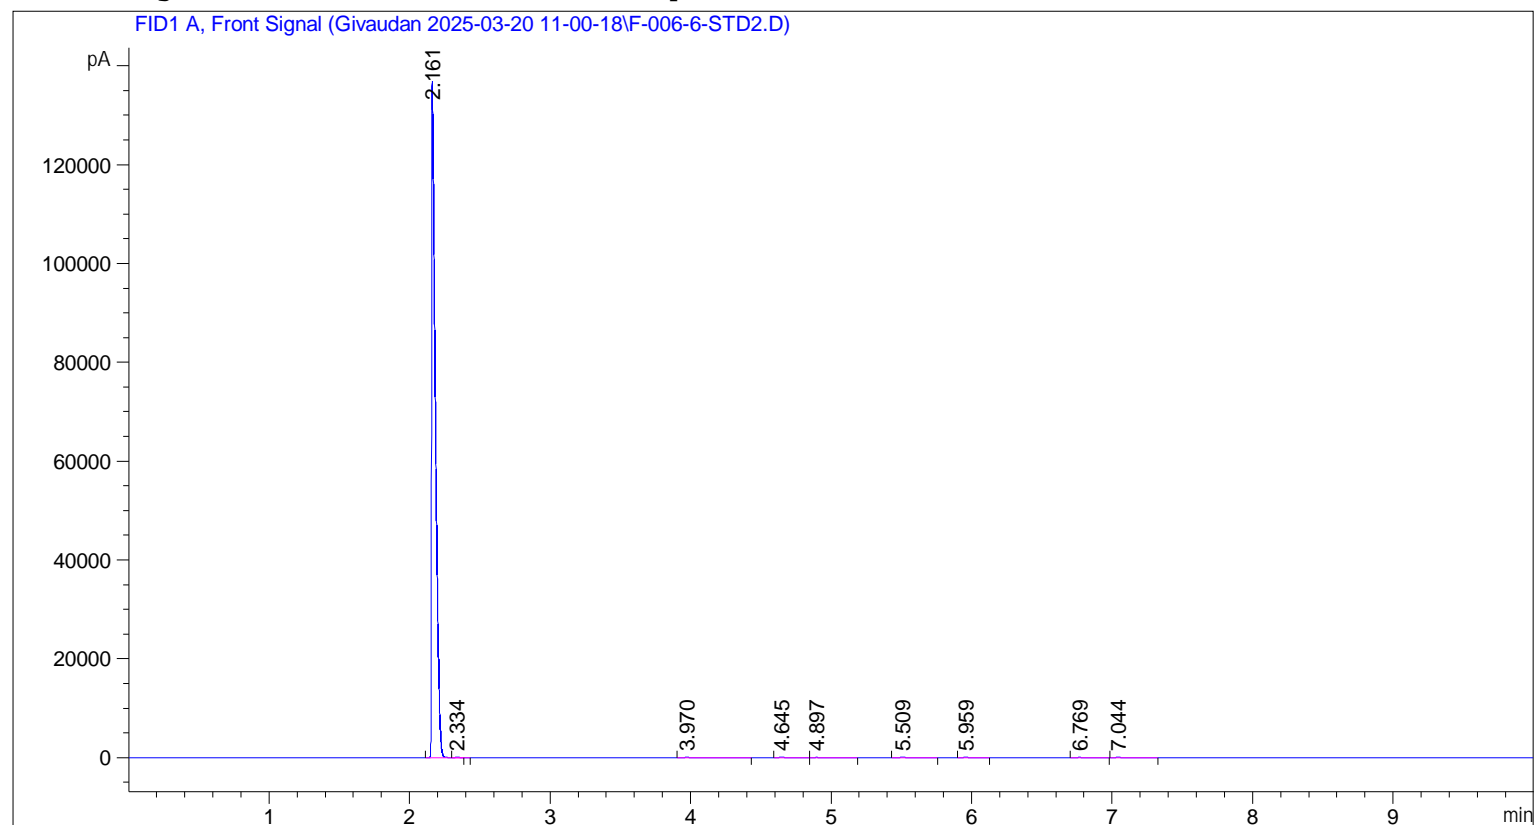Acq. Operator   : SYSTEM   Seq. Line :   6
Sample Operator : SYSTEM
Acq. Instrument : 8890GC   Location :   6 (F)
Injection Date : 3/20/2025 12:02:22 PM   Inj :   1
                                                Inj Volume : 1 µl
Method   : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-20 11-00-18
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed   : 2/14/2025 10:41:17 AM by SYSTEM

===
                        Area Percent Report
===

Sorted By   :   Signal
Calib. Data Modified :   9/13/2021 3:53:03 PM
Multiplier   :   1.0000
Dilution   :   1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A, Front Signal

Peak RetTime Type   Width   Area   Area   Name
  #   [min]   [min]   [pA*s]   %
----|-------|------|-------|----------|--------|--------------------
   1   2.161 BB S   0.0271 2.55647e5 99.73108 ?
   2   2.334 BB T   0.0304   59.41138 0.02318 ?
   3   3.970 BB   0.0447 100.64718 0.03926 Acetate
   4   4.645 BV   0.0346 119.39163 0.04658 Propionate
   5   4.897 VB   0.0327   53.22486 0.02076 Isobutyrate
   6   5.509 BB   0.0339 114.18723 0.04455 Butyrate
   7   5.959 BB   0.0335   83.19404 0.03246 Isovaleric
   8   6.769 BB   0.0351   64.72180 0.02525 Valeric

8890GC 3/20/2025 12:25:42 PM SYSTEM   Page   1 of 2

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.044	BB	0.0331	94.54974	0.03689	InternalSD

Totals :   2.56336e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                        *** End of Report ***