Data File C:\Users\P...uments\ChemStation\2\Data\std 2025-04-16 15-15-06\F-026-26-S7-5-1.D
Sample Name: S7-5-1

```
========================================================================
Acq. Operator   : SYSTEM                        Seq. Line :  26
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   26  (F)
Injection Date  : 4/16/2025 7:59:46 PM               Inj :    1
                                                Inj Volume : 1 µl
Sequence File   : C:\Users\Public\Documents\ChemStation\2\Data\std 2025-04-16 15-15-06\std.S
Method          : C:\Users\Public\Documents\ChemStation\2\Data\std 2025-04-16 15-15-06\SCFA_
                  FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
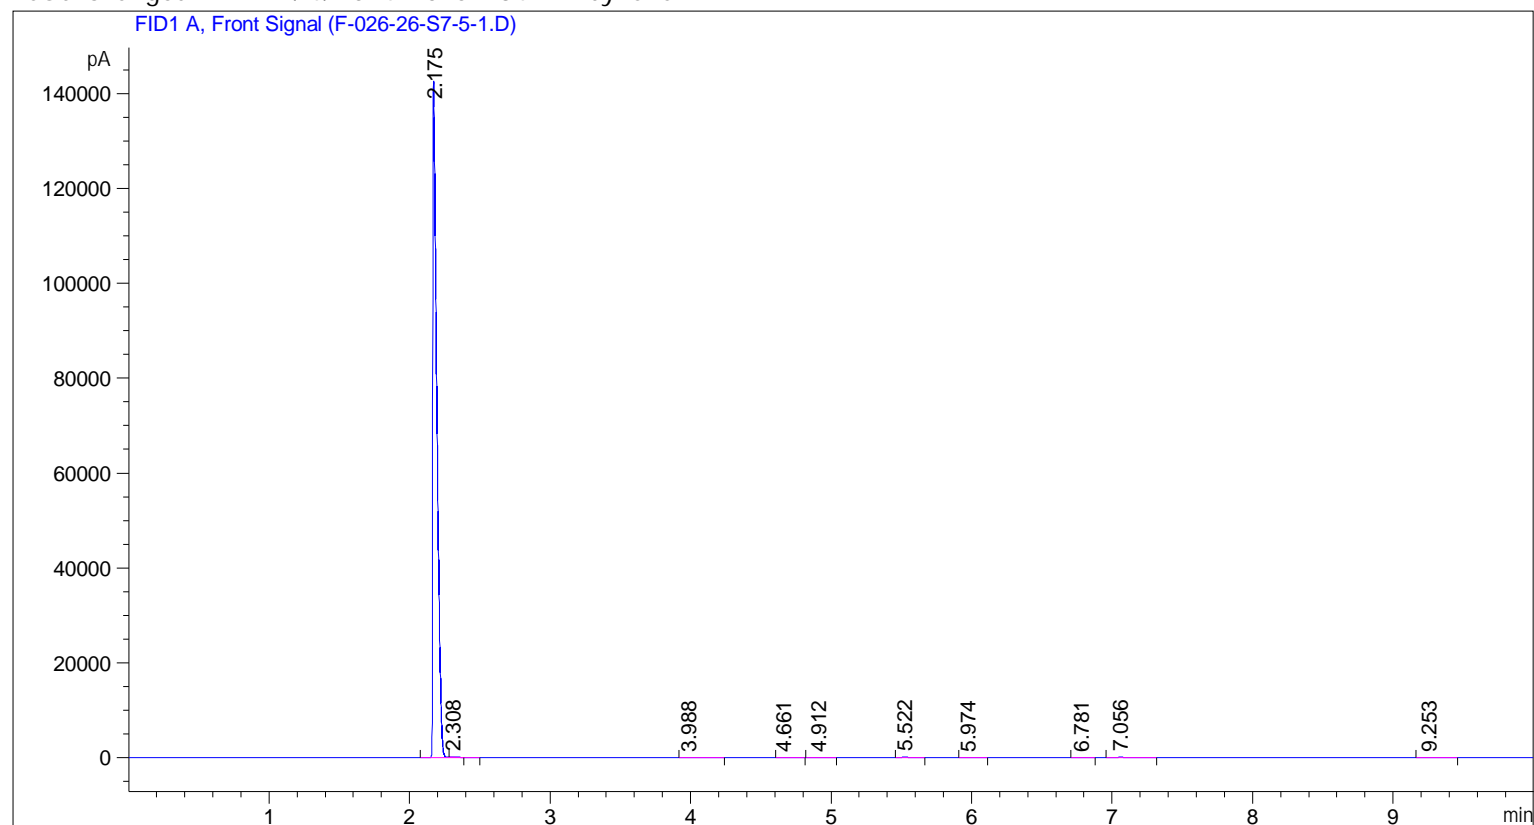


```
========================================================================
                        Area Percent Report
========================================================================
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

```
Peak RetTime  Type   Width     Area       Area     Name
 #   [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
  1   2.175 BB S    0.0297 2.84292e5  99.83065 ?
  2   2.308 BB T    0.0403  115.15997  0.04044 ?
  3   3.988 BB      0.0449   38.94836  0.01368 Acetate
  4   4.661 BB      0.0374   41.70759  0.01465 Propionate
  5   4.912 BB      0.0355   12.04227  0.00423 Isobutyrate
  6   5.522 BB      0.0349  140.61752  0.04938 Butyrate
  7   5.974 BB      0.0365   22.19701  0.00779 Isovaleric
```

Sample Name: S7-5-1

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
8	6.781	BB	0.0341	8.59844	0.00302	Valeric
9	7.056	BB	0.0345	95.12525	0.03340	InternalSD
10	9.253	BB	0.0434	7.87345	0.00276	?

Totals :   2.84774e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                       *** End of Report ***