Data File C:\Users\P...ments\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30\F-006-6-D11.D
Sample Name: D11

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   6
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   6   (F)
Injection Date  : 2/28/2025 2:29:09 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
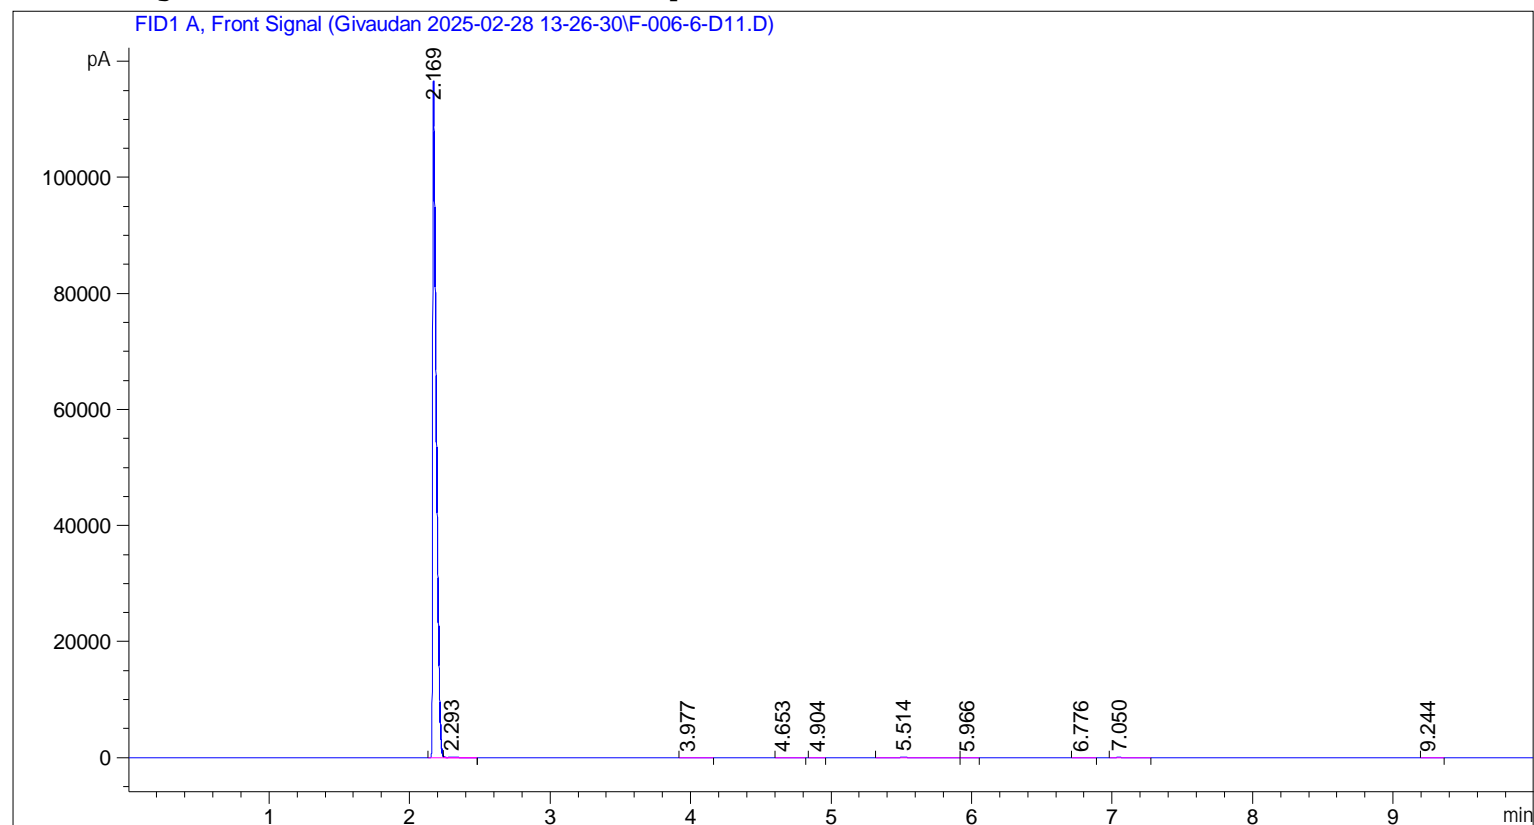

FID1 A, Front Signal (Givaudan 2025-02-28 13-26-30\F-006-6-D11.D)

```
=====================================================================
                      Area Percent Report
=====================================================================


Sorted By             :        Signal
Calib. Data Modified  :        9/13/2021 3:53:03 PM
Multiplier            :        1.0000
Dilution              :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area       Area      Name
  #   [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|---------------------
   1   2.169 BV R    0.0255 2.03111e5   99.64916 ?
   2   2.293 VB E    0.0417  292.74765   0.14363 ?
   3   3.977 BB      0.0373   43.08194   0.02114 Acetate
   4   4.653 BB      0.0348   40.05122   0.01965 Propionate
   5   4.904 BB      0.0319    7.33029   0.00360 Isobutyrate
   6   5.514 BB      0.0353  221.96432   0.10890 Butyrate
   7   5.966 BB      0.0344    9.58983   0.00470 Isovaleric
   8   6.776 BB      0.0352    9.32121   0.00457 Valeric
```

| Peak | RetTime | Type | Width | Area | Area | Name |
#	[min]		[min]	[pA*s]	%	
9	7.050	BB	0.0339	85.68292	0.04204	InternalSD
10	9.244	BB	0.0410	5.33618	0.00262	?

Totals :   2.03826e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                          *** End of Report ***