```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  18
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :  18  (F)
Injection Date  : 2/28/2025 4:45:05 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
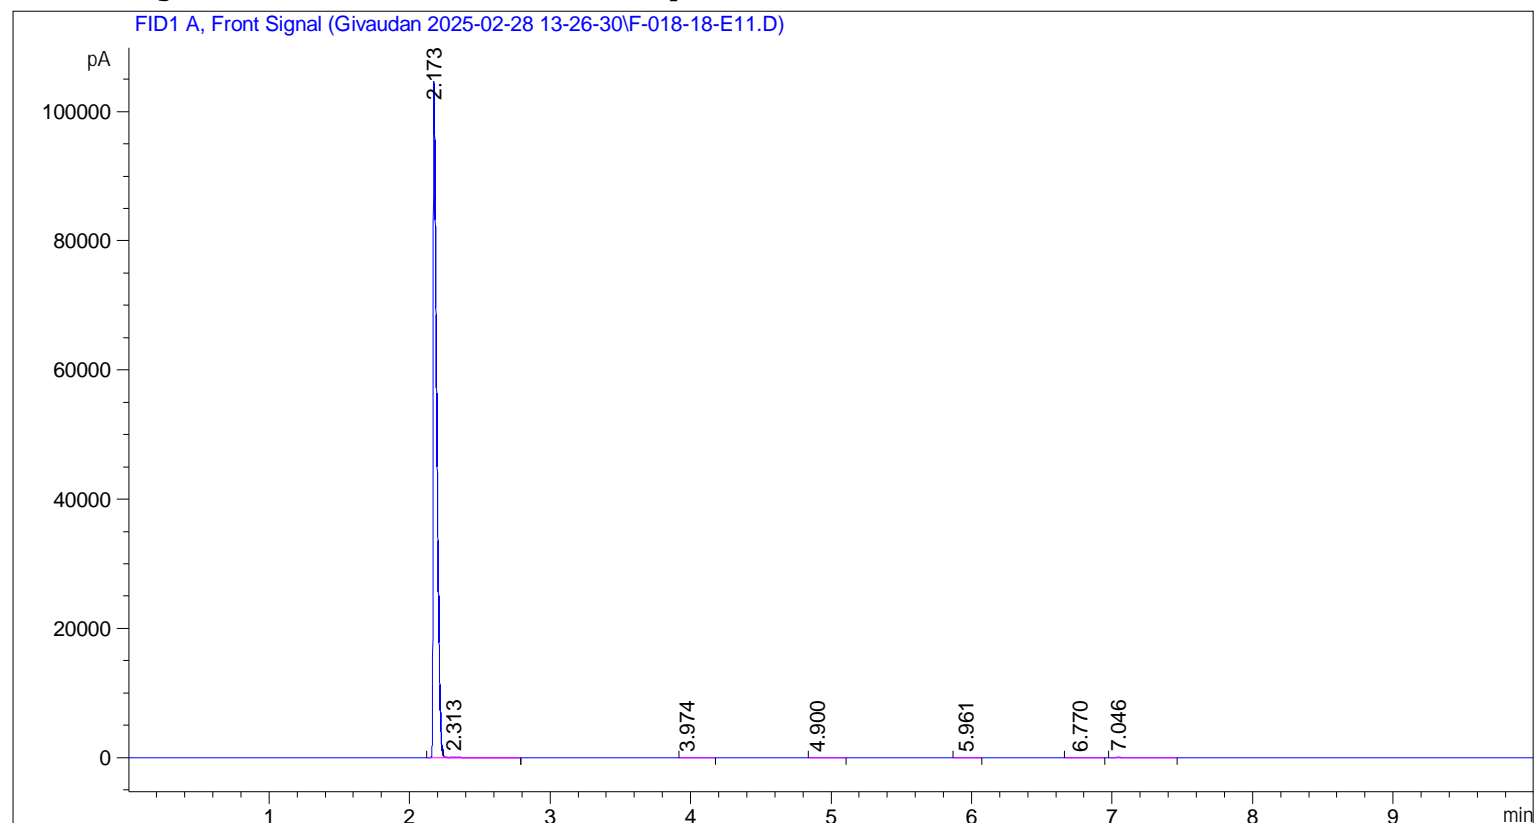

FID1 A, Front Signal (Givaudan 2025-02-28 13-26-30\F-018-18-E11.D)

```
=====================================================================
                    Area Percent Report
=====================================================================


Sorted By             :        Signal
Calib. Data Modified  :        9/13/2021 3:53:03 PM
Multiplier            :        1.0000
Dilution              :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area        Area     Name
  #   [min]          [min]   [pA*s]         %
----|-------|------|-------|----------|--------|--------------------
   1   2.173 BV R    0.0258 1.80694e5  99.75699 ?
   2   2.313 VB E    0.0687  339.03503  0.18717 ?
   3   3.974 BB      0.0390   19.21174  0.01061 Acetate
   4   4.725         0.0000    0.00000  0.00000 Propionate
   5   4.900 BB      0.0335    4.72754  0.00261 Isobutyrate
   6   5.598         0.0000    0.00000  0.00000 Butyrate
   7   5.961 BB      0.0341    5.52724  0.00305 Isovaleric
   8   6.770 BB      0.0455    7.07980  0.00391 Valeric
```

```
Peak RetTime  Type   Width     Area       Area     Name
  #   [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   9   7.046 BB      0.0348   64.58498  0.03566 InternalSD


Totals :                     1.81134e5
```

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                       *** End of Report ***