Data File C:\Users\P...\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16\F-003-3-GD_P1_A2.D
Sample Name: GD_P1_A2

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   3
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   3  (F)
Injection Date  : 1/22/2025 12:37:29 PM              Inj :   1
                                                Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-22 12-09-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
```
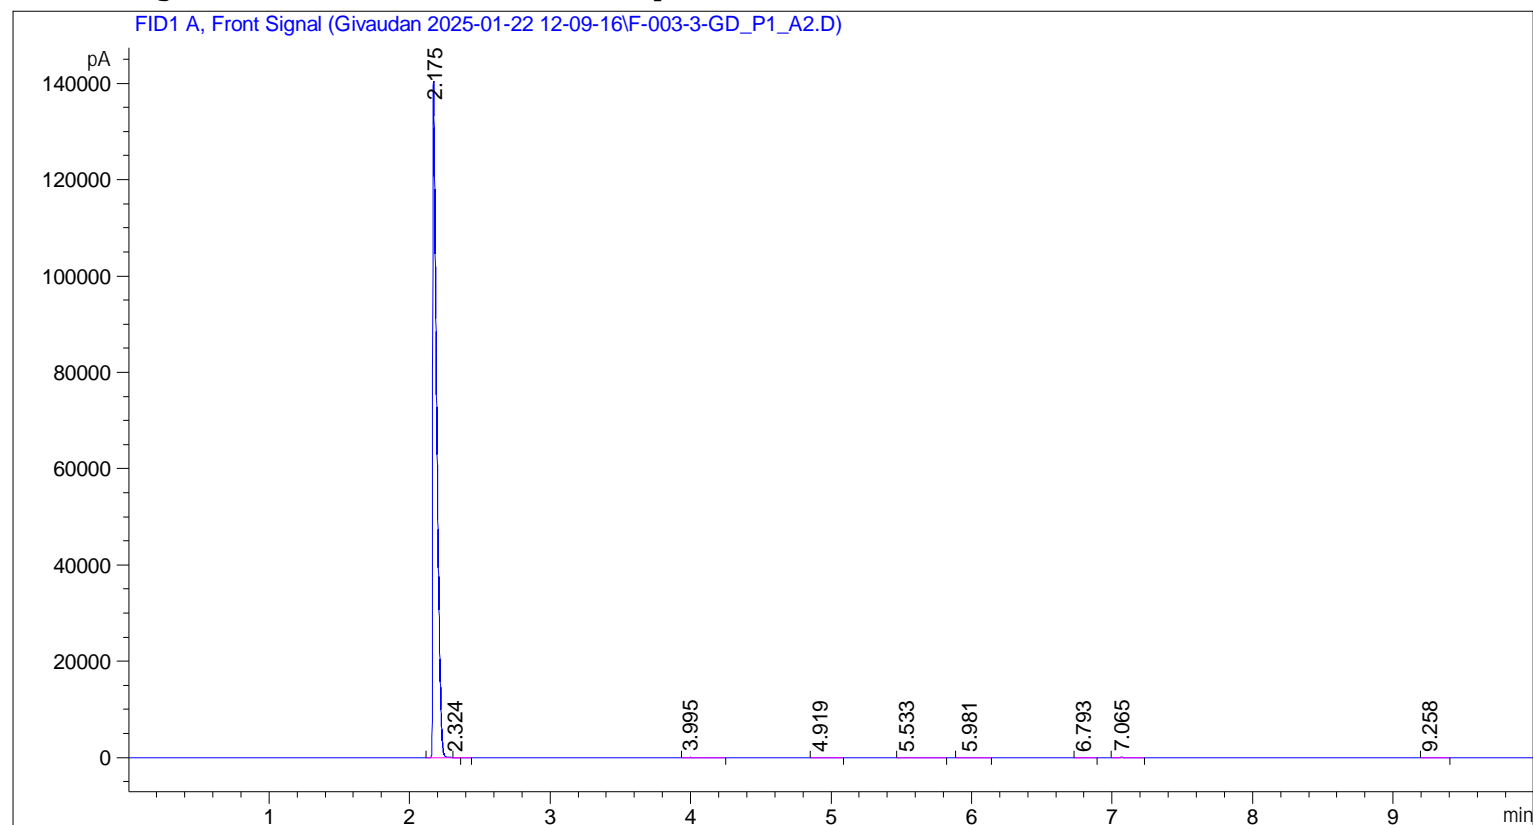

FID1 A, Front Signal (Givaudan 2025-01-22 12-09-16\F-003-3-GD_P1_A2.D)

```
=====================================================================
                        Area Percent Report
=====================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width      Area        Area      Name
  #   [min]          [min]    [pA*s]          %
----|-------|------|-------|----------|--------|--------------------
  1   2.175 BB S    0.0292 2.71136e5   99.92939 ?
  2   2.324 BB T    0.0316   12.06544   0.00445 ?
  3   3.995 BB      0.0430   69.91293   0.02577 Acetate
  4   4.725         0.0000    0.00000   0.00000 Propionate
  5   4.919 BB      0.0354    5.55992   0.00205 Isobutyrate
  6   5.533 BB      0.0357   21.39183   0.00788 Butyrate
  7   5.981 BB      0.0358    6.62176   0.00244 Isovaleric
  8   6.793 BB      0.0364    5.79389   0.00214 Valeric
```

```
  Peak RetTime  Type   Width     Area       Area      Name
   #   [min]          [min]   [pA*s]       %
----|-------|------|-------|----------|--------|--------------------
    9   7.065 BB     0.0346   65.78850  0.02425 InternalSD
   10   9.258 BB     0.0377    4.45436  0.00164 ?


 Totals :                    2.71327e5



 2 Warnings or Errors :

 Warning : Calibration warnings (see calibration table listing)
 Warning : Calibrated compound(s) not found

 ======================================================================
                        *** End of Report ***
```