


```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    6
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                     Location  :    6 (F)
Injection Date  : 1/23/2025 4:44:35 PM        Inj       :    1
                                           Inj Volume: 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-01-23 15-46-16
                  \SCFA_FrontOnly_053024.M (Sequence Method)
Last changed    : 7/4/2024 10:51:34 AM by SYSTEM
=====
```

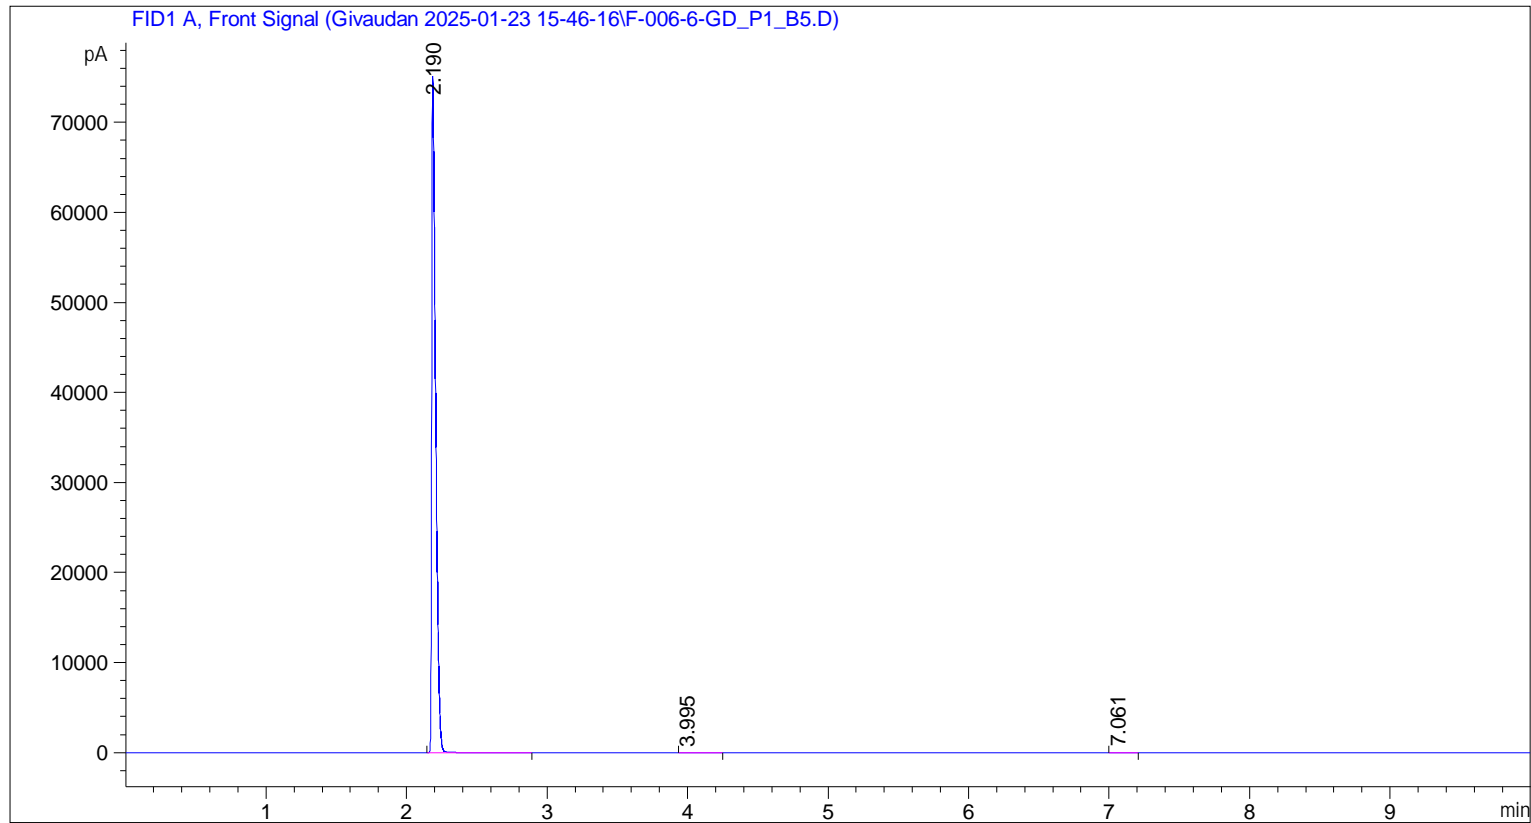

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.190	BB	0.0284	1.44987e5	99.97033	?
2	3.995	BB	0.0428	16.19180	0.01116	Acetate
3	4.725		0.0000	0.00000	0.00000	Propionate
4	4.978		0.0000	0.00000	0.00000	Isobutyrate
5	5.598		0.0000	0.00000	0.00000	Butyrate
6	6.050		0.0000	0.00000	0.00000	Isovaleric
7	6.869		0.0000	0.00000	0.00000	Valeric
8	7.061	BB	0.0334	26.83676	0.01850	InternalSD

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
----	-----	-----	-----	-----	-----	-----
Totals :				1.45030e5		

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*