


```
=====
Acq. Operator   : SYSTEM                      Seq. Line :   69
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                     Location  :   69   (F)
Injection Date  : 3/4/2025 12:17:43 AM        Inj       :    1
                                           Inj Volume: 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
=====
```

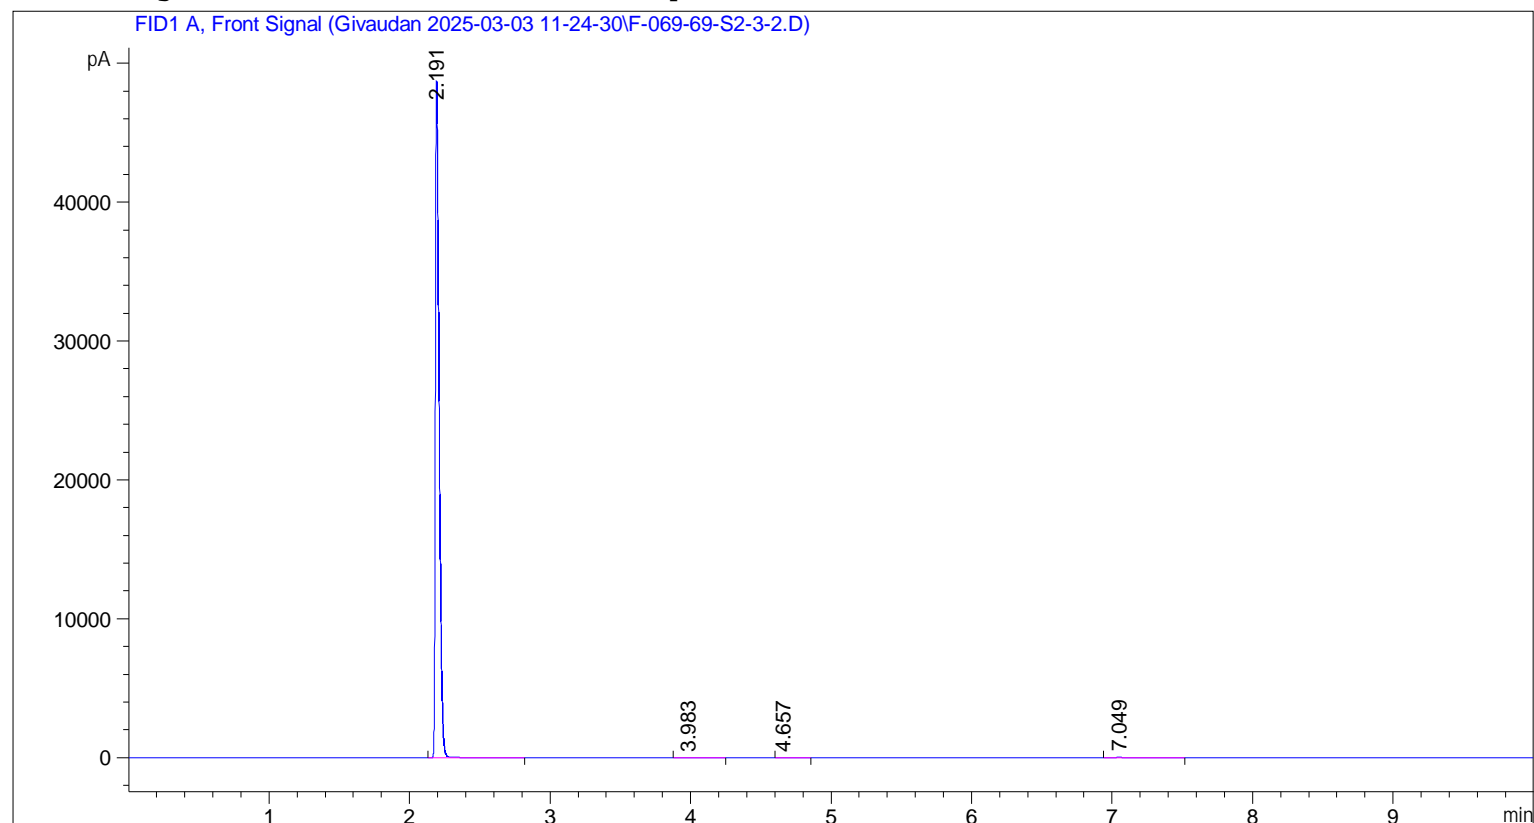

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.191	BB	0.0281	9.03750e4	99.92977	?
2	3.983	BB	0.0431	13.42178	0.01484	Acetate
3	4.657	BB	0.0420	8.79908	0.00973	Propionate
4	4.978		0.0000	0.00000	0.00000	Isobutyrate
5	5.598		0.0000	0.00000	0.00000	Butyrate
6	6.050		0.0000	0.00000	0.00000	Isovaleric
7	6.869		0.0000	0.00000	0.00000	Valeric
8	7.049	BB	0.0410	41.29176	0.04566	InternalSD

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
----- ----- ----- ----- ----- ----- -----						
Totals :				9.04385e4		

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*