```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  10
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :   10  (F)
Injection Date  : 2/11/2025 5:15:02 PM                  Inj :   1
                                                 Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-11 15-31-38
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/11/2025 3:11:07 PM by SYSTEM
```
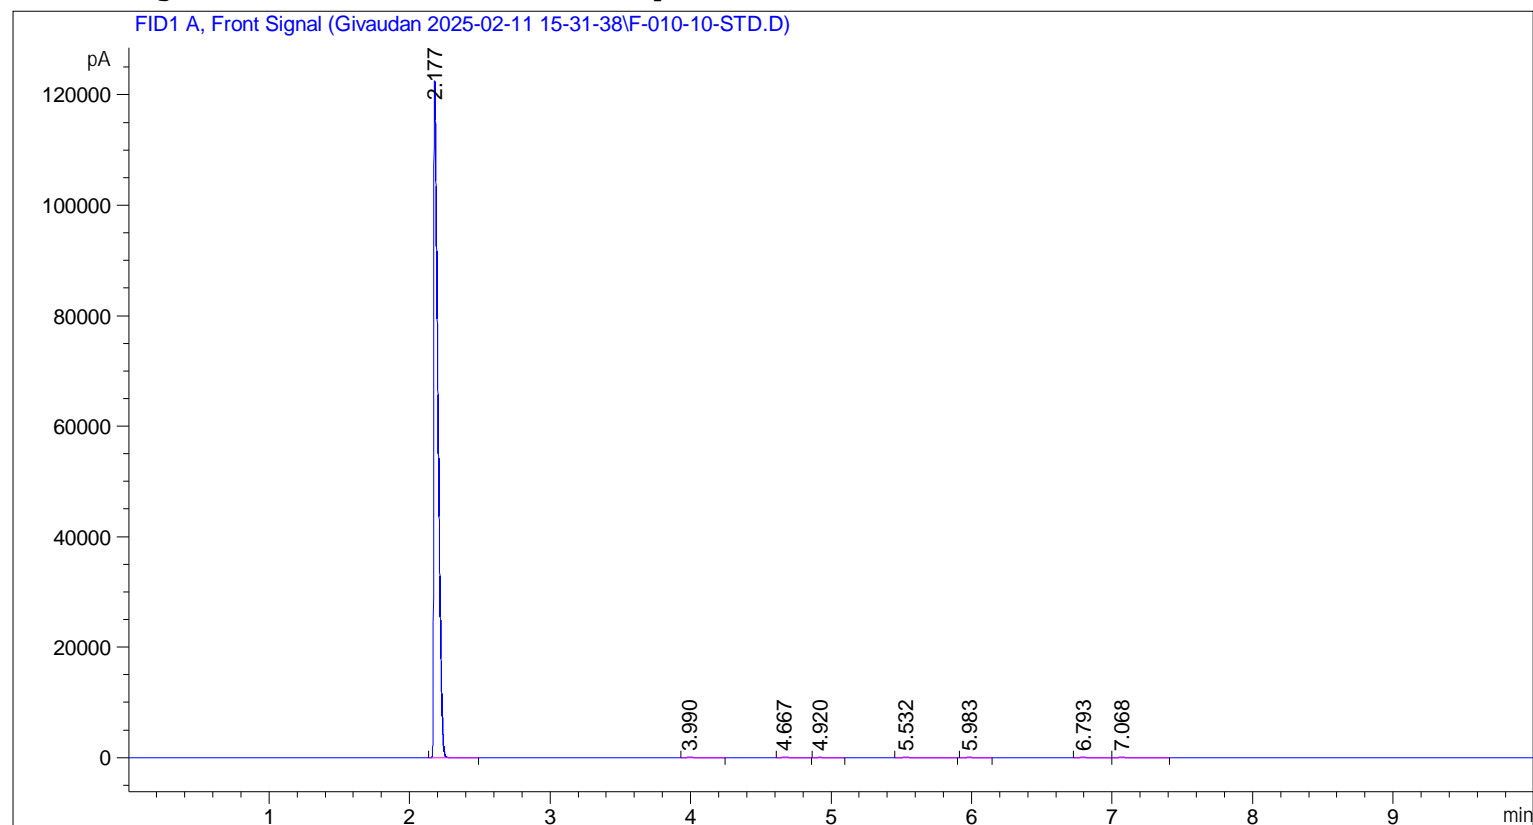


```
=====================================================================
                    Area Percent Report
=====================================================================


Sorted By             :      Signal
Calib. Data Modified  :      9/13/2021 3:53:03 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal

Peak RetTime  Type   Width     Area       Area      Name
  #   [min]          [min]    [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   2.177 BB      0.0321 2.50832e5  99.64581 ?
   2   3.990 BB      0.0393  130.26025  0.05175 Acetate
   3   4.667 BB      0.0362  168.49870  0.06694 Propionate
   4   4.920 BB      0.0346   59.43917  0.02361 Isobutyrate
   5   5.532 BB      0.0354  164.38943  0.06531 Butyrate
   6   5.983 BB      0.0343  103.74064  0.04121 Isovaleric
   7   6.793 BB      0.0355  105.32355  0.04184 Valeric
   8   7.068 BB      0.0344  159.93393  0.06354 InternalSD
```

```
   Peak RetTime  Type   Width     Area       Area     Name
    #   [min]          [min]   [pA*s]        %
   ----|-------|------|-------|----------|--------|--------------------
   Totals :                   2.51724e5
```

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

===
                         *** End of Report ***