


```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    1
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                     Location  :    1 (F)
Injection Date  : 3/3/2025 11:27:17 AM        Inj       :    1
                                           Inj Volume: 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
=====
```

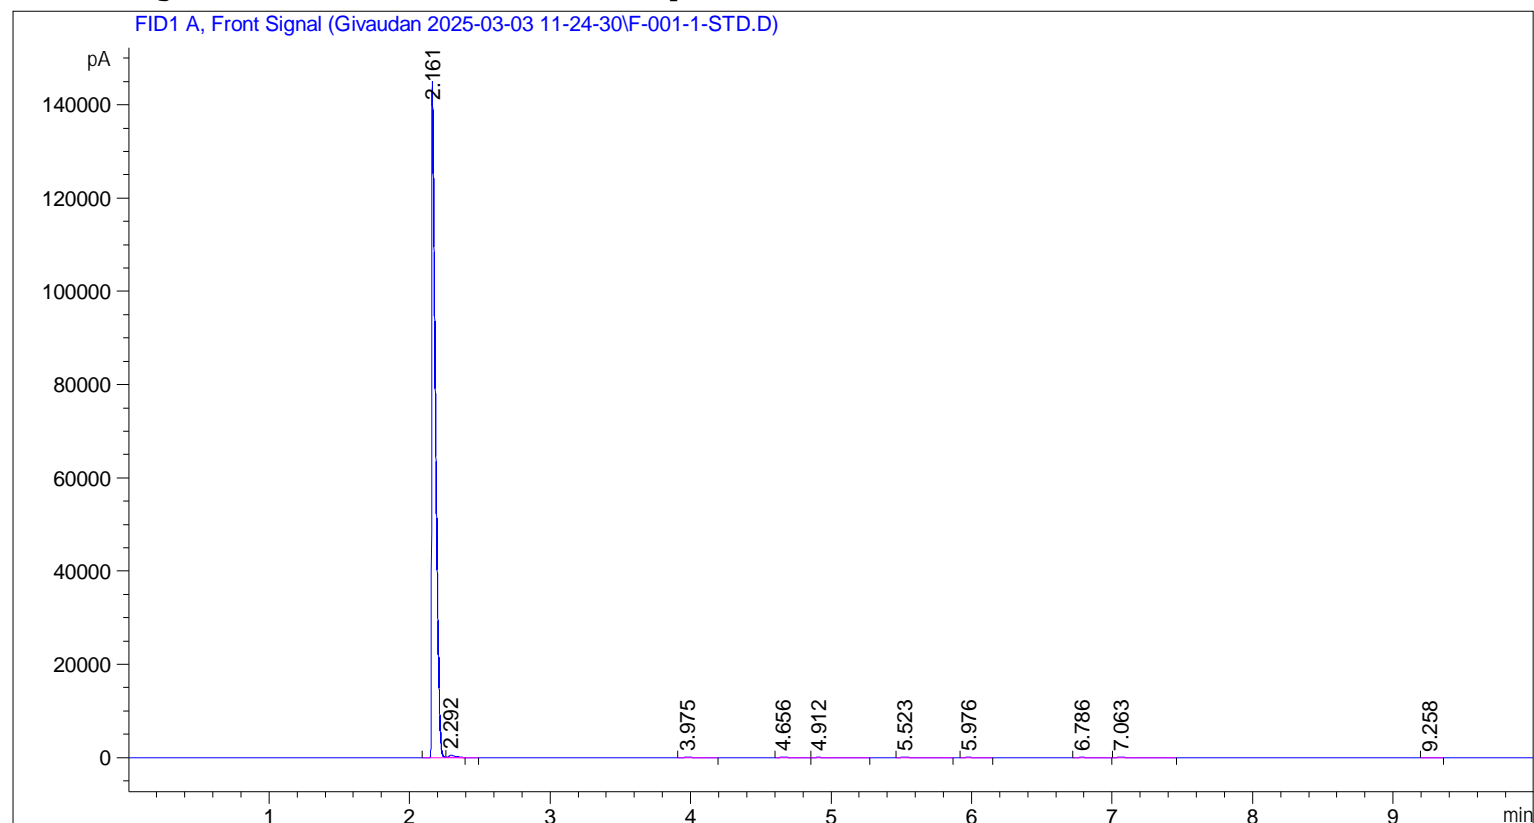

```
=====
                          Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      9/13/2021 3:53:03 PM
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.161	BB S	0.0276	2.68357e5	98.87066	?
2	2.292	BB T	0.0451	1439.87378	0.53049	?
3	3.975	BB	0.0372	245.16483	0.09033	Acetate
4	4.656	BV	0.0349	318.06833	0.11719	Propionate
5	4.912	VB	0.0331	104.10371	0.03835	Isobutyrate
6	5.523	BB	0.0349	342.81778	0.12630	Butyrate
7	5.976	BB	0.0327	148.70004	0.05479	Isovaleric
8	6.786	BB	0.0350	130.92462	0.04824	Valeric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.063	BB	0.0331	328.13345	0.12089	InternalSD
10	9.258	BB	0.0383	7.50088	0.00276	?

Totals : 2.71422e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====
*** End of Report ***