```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   2
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                         Location :   2  (F)
Injection Date  : 3/3/2025 11:38:37 AM               Inj :   1
                                                Inj Volume : 1 µl
Method            : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-03-03 11-24-30
                    \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
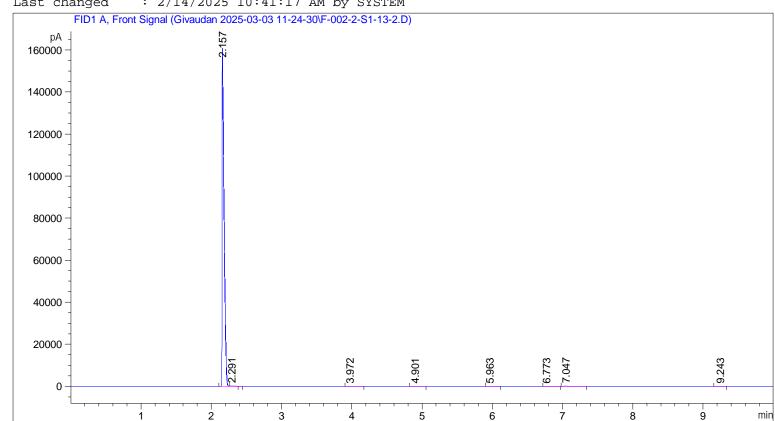

FID1 A, Front Signal (Givaudan 2025-03-03 11-24-30\F-002-2-S1-13-2.D)

```
=====================================================================
                     Area Percent Report
=====================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.157	BB S	0.0284	3.06130e5	99.80049	?
2	2.291	BB T	0.0456	320.15445	0.10437	?
3	3.972	BB	0.0389	45.44610	0.01482	Acetate
4	4.725		0.0000	0.00000	0.00000	Propionate
5	4.901	BB	0.0349	8.95752	0.00292	Isobutyrate
6	5.598		0.0000	0.00000	0.00000	Butyrate
7	5.963	BB	0.0343	10.72625	0.00350	Isovaleric
8	6.773	BB	0.0360	9.83986	0.00321	Valeric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.047	BB	0.0343	208.64427	0.06802	InternalSD
10	9.243	BB	0.0388	8.22406	0.00268	?

Totals :   3.06742e5

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found

===
                         *** End of Report ***