```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :  14
Sample Operator : SYSTEM
Acq. Instrument : 8890GC                           Location :  14  (F)
Injection Date  : 2/28/2025 3:59:48 PM                 Inj :  1
                                                  Inj Volume : 1 µl
Method          : C:\Users\Public\Documents\ChemStation\2\Data\Givaudan 2025-02-28 13-26-30
                  \SCFA_FrontOnly_082321.M (Sequence Method)
Last changed    : 2/14/2025 10:41:17 AM by SYSTEM
```
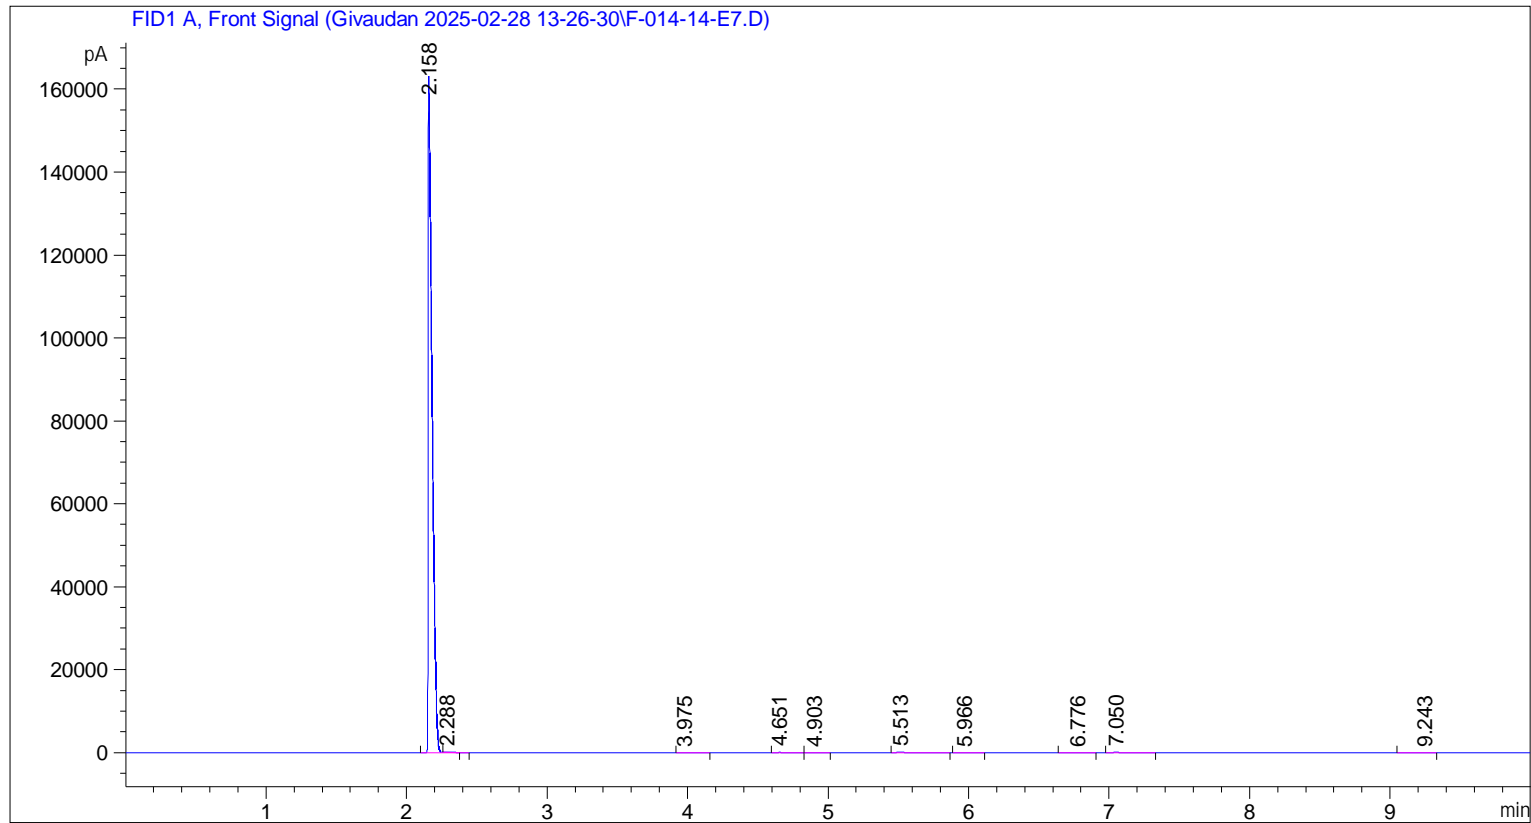

FID1 A, Front Signal (Givaudan 2025-02-28 13-26-30\F-014-14-E7.D)

```
=====================================================================
                      Area Percent Report
=====================================================================


Sorted By            :        Signal
Calib. Data Modified :        9/13/2021 3:53:03 PM
Multiplier           :        1.0000
Dilution             :        1.0000
Do not use Multiplier & Dilution Factor with ISTDs



Signal 1: FID1 A, Front Signal
```

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	2.158	BB S	0.0285	3.12135e5	99.68191	?
2	2.288	BB T	0.0398	359.24033	0.11473	?
3	3.975	BB	0.0380	56.27242	0.01797	Acetate
4	4.651	BB	0.0354	68.42039	0.02185	Propionate
5	4.903	BB	0.0338	10.85056	0.00347	Isobutyrate
6	5.513	BB	0.0340	306.52896	0.09789	Butyrate
7	5.966	BB	0.0358	14.67344	0.00469	Isovaleric
8	6.776	BB	0.0366	13.56949	0.00433	Valeric

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
9	7.050	BB	0.0334	121.49454	0.03880	InternalSD
10	9.243	BB	0.0810	44.98928	0.01437	?

Totals :   3.13131e5

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

==
                         *** End of Report ***