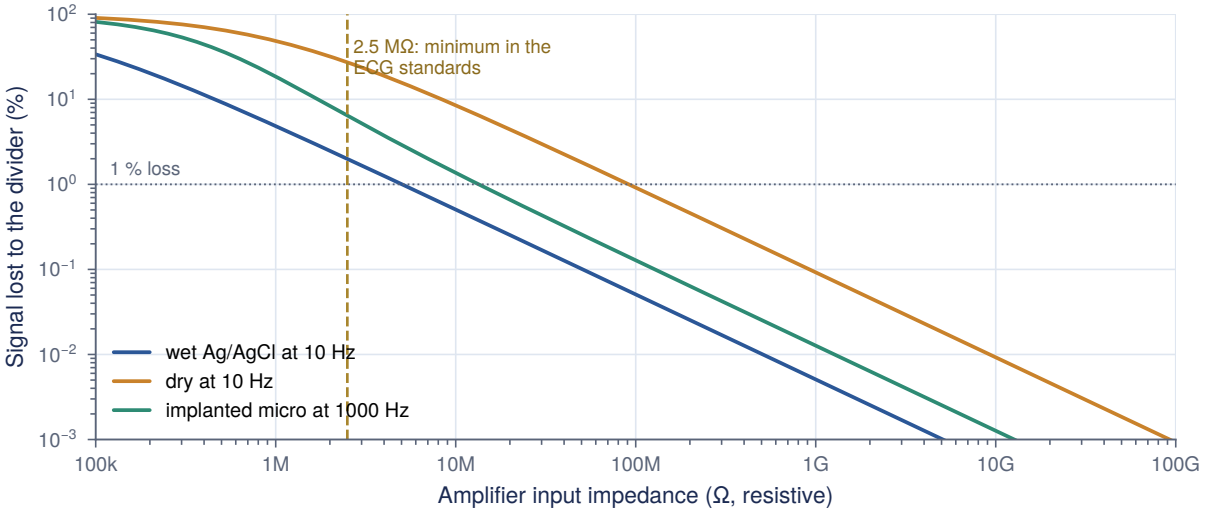
2.5 MΩ: minimum in the
ECG standards
1 % loss
wet Ag/AgCl at 10 Hz
dry at 10 Hz
implanted micro at 1000 Hz
Signal lost to the divider (%)
Amplifier input impedance (Ω, resistive)
10^{2}
10^{1}
10^{0}
10^{-1}
10^{-2}
10^{-3}
100k
1M
10M
100M
1G
10G
100G