~ Calibration Certificate ~

Per ISO 16063-21

Model Number: 352B01

Serial Number: 256964

Description: ICP® Accelerometer

Manufacturer: PCB

Method: Back-to-Back Comparison AT401-3

Calibration Data

Sensitivity @ 100 Hz	**0.979 mV/g**	Output Bias	10.9 VDC
	(0.0999 mV/m/s²)	Transverse Sensitivity	1.5 %
Resonant Frequency	109.9 kHz		

Sensitivity Plot

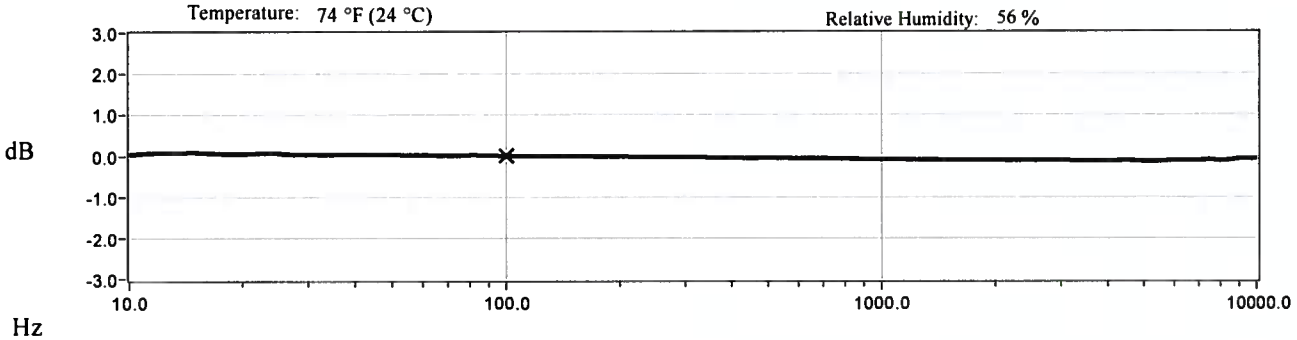

Data Points

Frequency (Hz)	Dev. (%)	Frequency (Hz)	Dev. (%)	Frequency (Hz)	Dev. (%)
10	0.4	300	-0.4	7000	-1.3
15	0.9	500	-0.7	10000	-0.9
30	0.3	1000	-1.1		
50	0.3	3000	-1.4		
REF. FREQ.	0.0	5000	-1.6		

Mounting Surface: Tungsten Adapter Fastener: Adhesive Fixture Orientation: Vertical
Acceleration Level (pk)[1]: 10.0 g (98.1 m/s²)
[1]The acceleration level may be limited by shaker displacement at low frequencies. If the listed level cannot be obtained, the calibration system uses the following formula to set the vibration amplitude; Acceleration Level (g) = 0.008 x (freq)². [2]The gravitational constant used for calculations by the calibration system is; 1 g = 9.80665 m/s².

Condition of Unit

As Found: n/a

As Left: New Unit, In Tolerance

Notes

1. Calibration is NIST Traceable thru Project 683/287323 and PTB Traceable thru Project 17014.
2. This certificate shall not be reproduced, except in full, without written approval from PCB Piezotronics, Inc.
3. Calibration is performed in compliance with ISO 10012-1, ANSI Z540.3 and ISO 17025.
4. See Manufacturer's Specification Sheet for a detailed listing of performance specifications.
5. Measurement uncertainty (95% confidence level with coverage factor of 2) for frequency ranges tested during calibration are as follows: 5-9 Hz; +/- 2.0%, 10-99 Hz; +/- 1.5%, 100-1999 Hz; +/- 1.0%, 2-10 kHz; +/- 2.5%.

Technician: Richard Gardner RG Date: 10/4/2018

ACCREDITED
CALIBRATION CERT #1862.01

PCB PIEZOTRONICS INC.
VIBRATION DIVISION
3425 Walden Avenue · Depew, NY 14043
TEL: 888-684-0013 · FAX: 716-685-3886 · www.pcb.com

CAL63-3621497431.610+0

ACS-1