

~ Calibration Certificate ~

Per ISO 16063-21

247393

Model Number: 352B01

Serial Number: 247393

Description: ICP® Accelerometer

Manufacturer: PCB


Method: Back-to-Back Comparison AT401-3

Calibration Data

Sensitivity @ 100 Hz 0.936 mV/g
(0.0954 mV/m/s²)
Resonant Frequency 119.5 kHz

Output Bias 10.0 VDC
Transverse Sensitivity 1.0 %

Sensitivity Plot

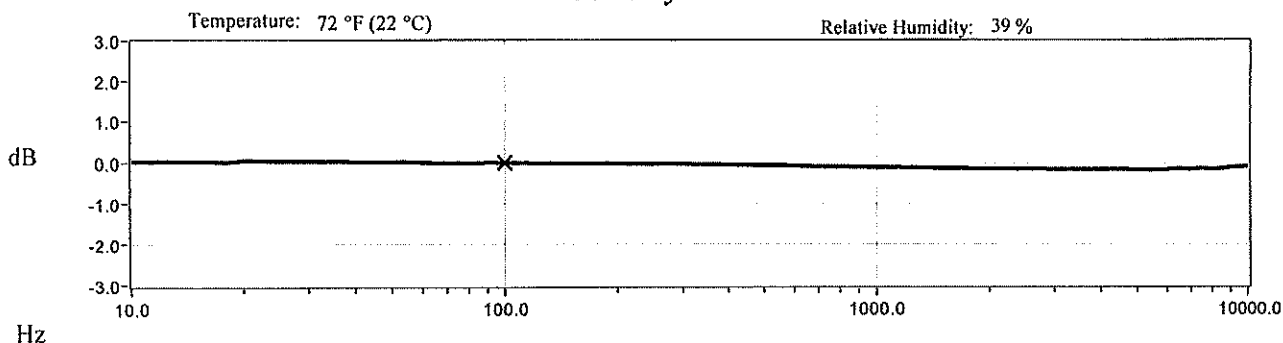

Data Points

Frequency (Hz)	Dev. (%)	Frequency (Hz)	Dev. (%)	Frequency (Hz)	Dev. (%)
10	0.2	300	-0.4	7000	-1.9
15	0.3	500	-0.8	10000	-1.0
30	0.3	1000	-1.3		
50	0.2	3000	-1.8		
REF. FREQ.	0.0	5000	-1.9		

Mounting Surface: Tungsten Adapter Fastener: Adhesive Fixture Orientation: Vertical

Acceleration Level (pk): 10.0 g (98.1 m/s²)

*The acceleration level may be limited by shaker displacement at low frequencies. If the listed level cannot be obtained, the calibration system uses the following formula to set the vibration amplitude: Acceleration Level (g) = 0.008 x (freq)^{1.5}. *The gravitational constant used for calculations by the calibration system is: 1 g = 9.80665 m/s².

Condition of Unit

As Found: n/a

As Left: New Unit, In Tolerance

Notes

1. Calibration is NIST Traceable thru Project 683/287323 and PTB Traceable thru Project 17014.
2. This certificate shall not be reproduced, except in full, without written approval from PCB Piezotronics, Inc.
3. Calibration is performed in compliance with ISO 10012-1, ANSI/NCSS Z540-1-1994 and ISO 17025.
4. See Manufacturer's Specification Sheet for a detailed listing of performance specifications.
5. Measurement uncertainty (95% confidence level with coverage factor of 2) for frequency ranges tested during calibration are as follows: 5-9 Hz; +/- 2.0%, 10-99 Hz; +/- 1.5%, 100-1999 Hz; +/- 1.0%, 2-10 kHz; +/- 2.5%.

Technician: Mike Ferrio MAF

Date: 3/17/2018



CALIBRATION CERT #1862.01

PAGE 1 of 1

PCB PIEZOTRONICS
VIBRATION DIVISION

3425 Walden Avenue Depew, NY 14043

TEL: 888-684-0013 FAX: 716-685-3886 www.pcb.com

CAL4-3604133886,553+0

