

# ~ Calibration Certificate ~

Per ISO 16063-21

Model Number: 352B01

Serial Number: 256965

Description: ICP® Accelerometer


Manufacturer: PCB

Method: Back-to-Back Comparison AT401-3

## Calibration Data

Sensitivity @ 100 Hz      0.955 mV/g      Output Bias      10.1 VDC  
(0.0974 mV/m/s<sup>2</sup>)      Transverse Sensitivity      0.6 %  
Resonant Frequency      101.1 kHz

## Sensitivity Plot

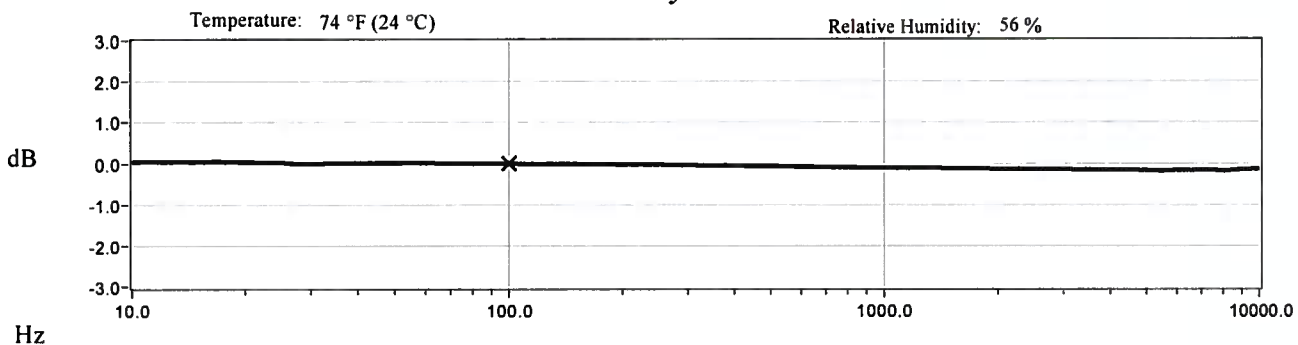

## Data Points

| Frequency (Hz) | Dev. (%) | Frequency (Hz) | Dev. (%) | Frequency (Hz) | Dev. (%) |
|----------------|----------|----------------|----------|----------------|----------|
| 10             | 0.5      | 300            | -0.5     | 7000           | -1.9     |
| 15             | 0.4      | 500            | -0.8     | 10000          | -1.6     |
| 30             | -0.2     | 1000           | -1.3     |                |          |
| 50             | 0.1      | 3000           | -1.7     |                |          |
| REF. FREQ.     | 0.0      | 5000           | -2.0     |                |          |

Mounting Surface: Tungsten Adapter    Fastener: Adhesive    Fixture Orientation: Vertical

Acceleration Level (pk): 10.0 g (98.1 m/s<sup>2</sup>)

\*The acceleration level may be limited by shaker displacement at low frequencies. If the listed level cannot be obtained, the calibration system uses the following formula to set the vibration amplitude: Acceleration Level (g) = 0.008 x (freq)<sup>2</sup>. \*The gravitational constant used for calculations by the calibration system is: 1 g = 9.80665 m/s<sup>2</sup>.

## Condition of Unit

As Found: n/a

As Left: New Unit, In Tolerance

## Notes

1. Calibration is NIST Traceable thru Project 683/287323 and PTB Traceable thru Project 17014.
2. This certificate shall not be reproduced, except in full, without written approval from PCB Piezotronics, Inc.
3. Calibration is performed in compliance with ISO 10012-1, ANSI Z540.3 and ISO 17025.
4. See Manufacturer's Specification Sheet for a detailed listing of performance specifications.
5. Measurement uncertainty (95% confidence level with coverage factor of 2) for frequency ranges tested during calibration are as follows: 5-9 Hz; +/- 2.0%, 10-99 Hz; +/- 1.5%, 100-1999 Hz; +/- 1.0%, 2-10 kHz; +/- 2.5%.

Technician: Richard Gardner RJ

Date: 10/4/2018



CALIBRATION CERT #1862.01

**PCB PIEZOTRONICS**  
VIBRATION DIVISION

3425 Walden Avenue    Depew, NY 14043

TEL: 888-684-0013    FAX: 716-685-3886    www.pcb.com

PAGE 1 of 1

CAL63-3621497877.261+0

